

# DANI Chromatographic Products

- GC and GC/MS
- Automatic samplers for GC

**Архангельск** (8182)63-90-72  
**Астана** (7172)727-132  
**Астрахань** (8512)99-46-04  
**Барнаул** (3852)73-04-60  
**Белгород** (4722)40-23-64  
**Брянск** (4832)59-03-52  
**Владивосток** (423)249-28-31  
**Волгоград** (844)278-03-48  
**Вологда** (8172)26-41-59  
**Воронеж** (473)204-51-73  
**Екатеринбург** (343)384-55-89  
**Иваново** (4932)77-34-06  
**Ижевск** (3412)26-03-58  
**Казань** (843)206-01-48

**Калининград** (4012)72-03-81  
**Калуга** (4842)92-23-67  
**Кемерово** (3842)65-04-62  
**Киров** (8332)68-02-04  
**Краснодар** (861)203-40-90  
**Красноярск** (391)204-63-61  
**Курск** (4712)77-13-04  
**Липецк** (4742)52-20-81  
**Магнитогорск** (3519)55-03-13  
**Москва** (495)268-04-70  
**Мурманск** (8152)59-64-93  
**Набережные Челны** (8552)20-53-41  
**Нижний Новгород** (831)429-08-12  
**Новокузнецк** (3843)20-46-81

**Новосибирск** (383)227-86-73  
**Омск** (3812)21-46-40  
**Орел** (4862)44-53-42  
**Оренбург** (3532)37-68-04  
**Пенза** (8412)22-31-16  
**Пермь** (342)205-81-47  
**Ростов-на-Дону** (863)308-18-15  
**Рязань** (4912)46-61-64  
**Самара** (846)206-03-16  
**Санкт-Петербург** (812)309-46-40  
**Саратов** (845)249-38-78  
**Севастополь** (8692)22-31-93  
**Симферополь** (3652)67-13-56  
**Смоленск** (4812)29-41-54

**Сочи** (862)225-72-31  
**Ставрополь** (8652)20-65-13  
**Сургут** (3462)77-98-35  
**Тверь** (4822)63-31-35  
**Томск** (3822)98-41-53  
**Тула** (4872)74-02-29  
**Тюмень** (3452)66-21-18  
**Ульяновск** (8422)24-23-59  
**Уфа** (347)229-48-12  
**Хабаровск** (4212)92-98-04  
**Челябинск** (351)202-03-61  
**Череповец** (8202)49-02-64  
**Ярославль** (4852)69-52-93





**MASTER GC - Fast Gas Chromatograph**




## ... *FAST Gas Chromatograph*

**MASTER GC** dramatically **increases** the laboratory **productivity** decreasing the analysis run time while preserving chromatographic resolution:

- fastest oven heating rate (up to 140 °C/min)
- fast cooling time
- carrier gas pressure range up to 120 psi
- up to 1:10000 split ratio (*...or fast on-column injector..*)





# Fast GC application - PAHs

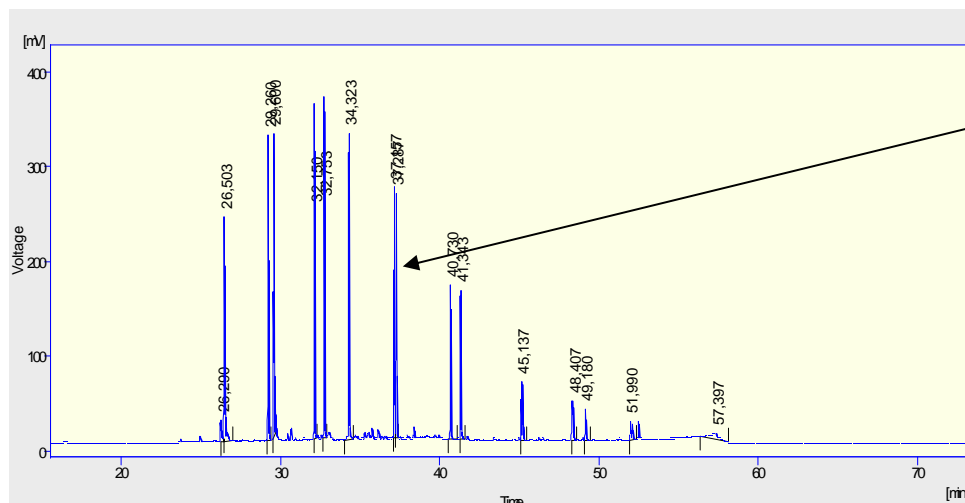

Conventional GC  
Rs = 1,48

Fast GC  
Rs = 1,35


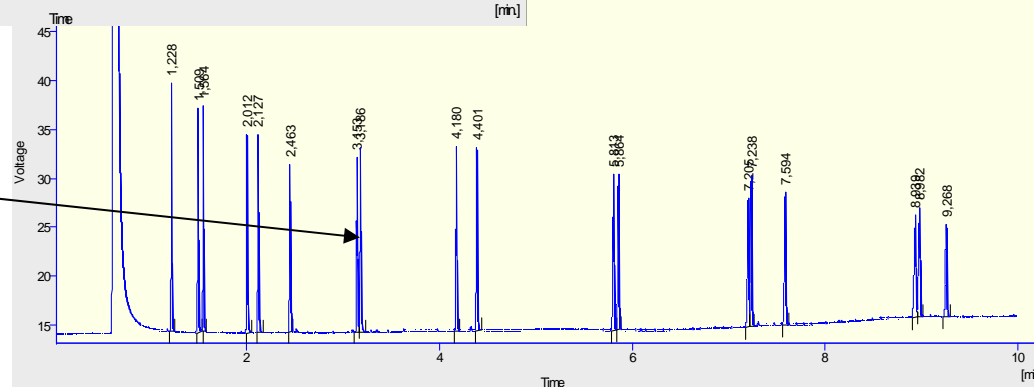



Column: DN-5, 15 m, 0.1 mm, 0.1 um; Oven: 140°C, 0.5min, 30°C/min, 220°C, 15°C/min, 300°C (1,5min); Carrier H2, 0.5mL/min, constant flow; Injector: PTV, 80°C-999°C/min-400°C; Split 1:100; Sample: 0.5µL

**6 times faster  
constant resolution**




## ... *Fast peak detection requirements*

- A fast response and data acquisition rate is necessary to properly detect fast peaks and avoid distortion in peak shape, peak height and apex location

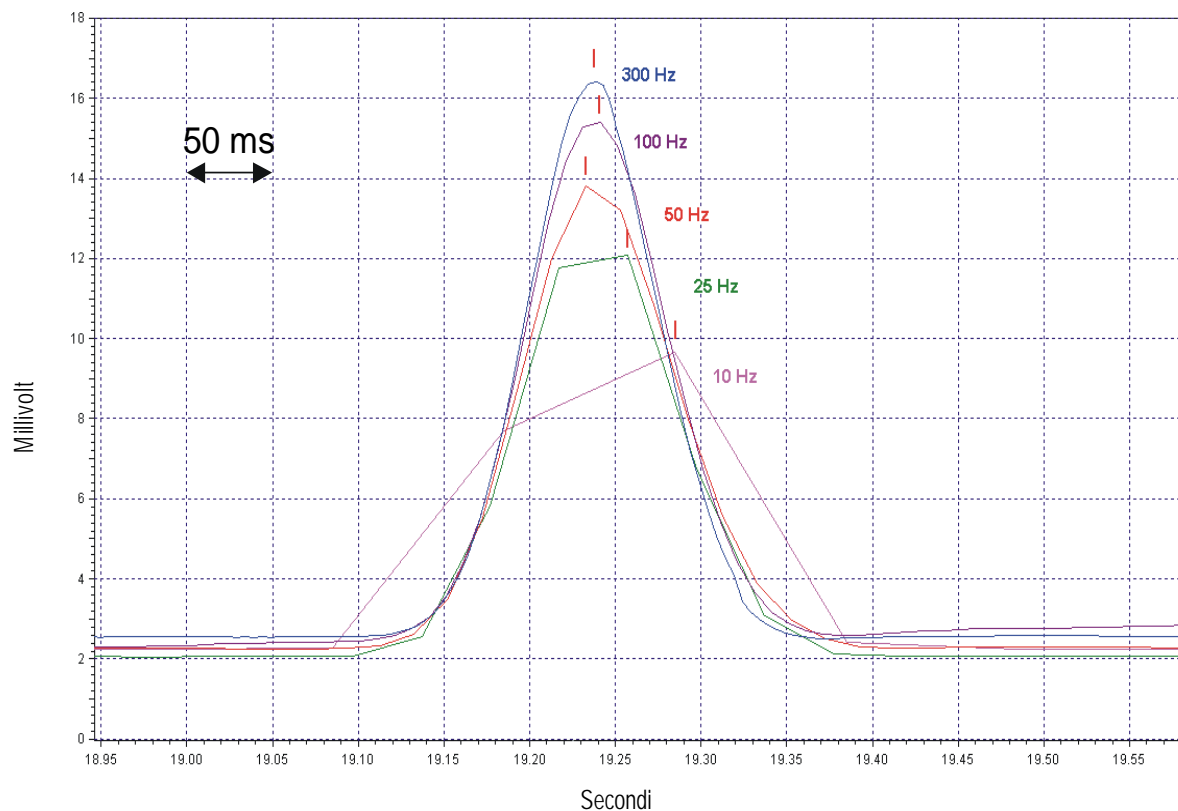

## ... full range of highly sensitive detectors

- MASTER GC features a full range of highly sensitive detectors.
- The digital setting of all the detector gas flow rates is included carrier
- A fast response and data acquisition rate up to 300 Hz for FID, ECD, NPD and FPD allows a reproducible and accurate acquisition also **of narrow fast GC peaks** keeping the sensitivity unaffected.

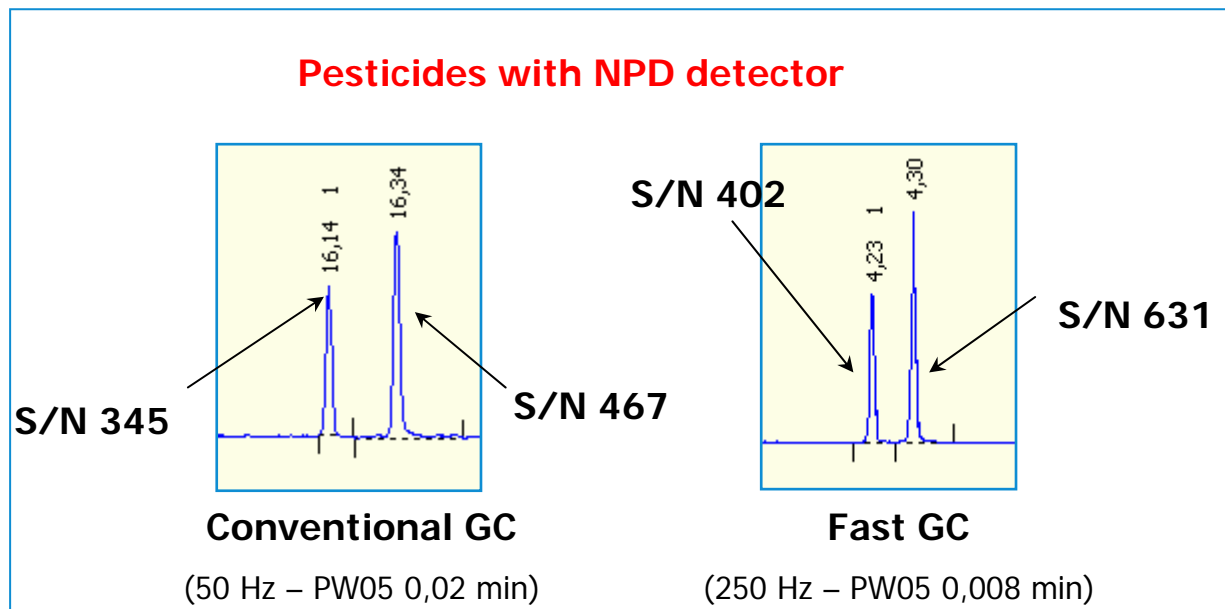


## ... unsurpassed repeatability

A patent pending Digital Flow Control (DFC) combined with a highly accurate control of the oven temperature assures an **unsurpassed retention time repeatability** and split flow **linearity** in both conventional and fast GC.

	C8	C10	C12	C14	C16	C18	C20	C22	C24	C26	C28
<b>1</b>	1,68	2,1905	2,6052	3,0072	3,4175	3,8249	4,2129	4,577	4,9161	5,2343	5,5505
<b>2</b>	1,6793	2,1892	2,6042	3,0072	3,4175	3,8249	4,2119	4,5757	4,9151	5,233	5,5495
<b>3</b>	1,6786	2,1888	2,6045	3,0075	3,4185	3,8259	4,2129	4,5767	4,9155	5,2343	5,5505
<b>4</b>	1,6803	2,1905	2,6052	3,0079	3,4182	3,8252	4,2133	4,577	4,9148	5,2326	5,5485
<b>5</b>	1,6786	2,1892	2,6038	3,0065	3,4172	3,8249	4,2126	4,576	4,9151	5,233	5,5485
<b>6</b>	1,6796	2,1902	2,6042	3,0065	3,4175	3,8245	4,2119	4,5763	4,9151	5,2336	5,5491
<b>7</b>	1,6793	2,1892	2,6042	3,0072	3,4175	3,8249	4,2119	4,5757	4,9151	5,233	5,5495
<b>8</b>	1,679	2,1888	2,6042	3,0072	3,4182	3,8249	4,2113	4,5757	4,9145	5,232	5,5475
<b>9</b>	1,6786	2,1898	2,6045	3,0062	3,4172	3,8245	4,2113	4,576	4,9148	5,2316	5,5485
<b>10</b>	1,6793	2,1898	2,6048	3,0075	3,4182	3,8255	4,2123	4,5757	4,9145	5,2323	5,5475
<b>Media</b>	1,6793	2,1896	2,6045	3,0071	3,4178	3,8250	4,2122	4,5762	4,9151	5,2330	5,5490
<b>Dev st</b>	<b>0,0006</b>	<b>0,0007</b>	<b>0,0005</b>	<b>0,0005</b>	<b>0,0005</b>	<b>0,0004</b>	<b>0,0007</b>	<b>0,0005</b>	<b>0,0005</b>	<b>0,0009</b>	<b>0,0011</b>



**RETENTION TIME REPEATABILITY**  
*SD < 0.001min*




<b>Oven Max Temperature</b>	500 °C
<b>Oven Max Heating Ramp Rate</b>	140°C/min
<b>Oven Temperature programming</b>	25 ramps, 26 isotherms
<b>Oven cool-down rate</b>	300°C to 50°C in 4 min
<b>Injectors installed simultaneously</b>	3
<b>Injectors available</b>	Packed (PK) Split/splitless (SL/IN) Programmable Temperature Vaporizer (PTV) Automated Fast On-Column Gas sampling valves (GSV)
<b>Injectors Gas Control (Carrier, Split, Purge)</b>	Digital Flow Control (DFC) Range: 0-120 psi
<b>Injector Pressure/Flow programming</b>	Constant or programmed flow Constant or programmed pressure Constant linear velocity Pulsed Injection Flow programming: 25 ramps/26 const. flows Pressure programming: 25 ramps/26 isobars Atmospheric pressure and temperature compensation







<b>Detectors installed simultaneously</b>	3
<b>Detectors available</b>	FID flame ionization detector NPD nitrogen and phosphorous detector ECD electron capture detector PID photo ionization detector TCD thermal conductivity detector mTCD micro thermal conductivity detector FPD flame photometric detector
<b>Detectors Gas Control</b>	Digital Pressure Control (DPC) Range: 0-120 psi
<b>Data Acquisition Rate</b>	300 Hz (for all detectors)
<b>GC User Interface</b>	Touch Screen - LCD TFT, 5.7"
<b>Output Signals</b>	Digital (LAN, USB, RS-232) Analog outputs (0-1V, 0-10V)
<b>Inside Oven Lamp</b>	YES



## MASTER AS – Automatic liquid Sampler

## ... maximized productivity


**MASTER AS** maximizes the laboratory productivity:

- **large sample capacity** (up to 160 vials)
- **extended capabilities** in injection techniques (sandwich injection, hot needle, internal standard, wide range of syringe volume..)
- **high flexibility** in the control of sample sequence (stored sample sequence, 25 lines, 100 repetitions, priority sequence, sensor for vial presence,..)


## ... with the highest accuracy and precision

**MASTER AS** assures a high degree of precision:



- RSD% area **repeatability** better than 0.3%
- outstanding sample volume **linearity**

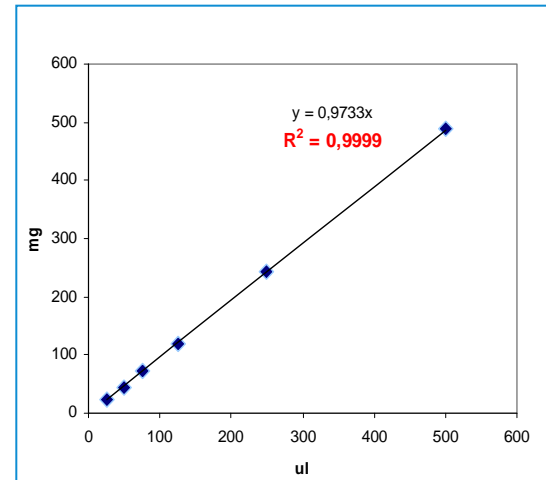

	C8	C10	C12	C14
1	188,749	157,419	102,825	101,723
2	188,317	156,319	102,568	101,577
3	187,259	155,916	101,847	101,07
4	187,479	156,438	101,89	101,644
5	188,231	156,458	102,241	102,004
6	188,108	156,314	102,214	101,828
7	188,109	156,861	102,165	101,956
8	188,024	156,89	101,859	101,196
9	188,73	156,865	102,498	101,875
10	188,891	156,833	102,431	101,771
11	188,518	157,469	102,749	101,401
<b>Media (mV.s)</b>	<b>188,220</b>	<b>156,707</b>	<b>102,299</b>	<b>101,640</b>
<b>SD</b>	<b>0,512</b>	<b>0,474</b>	<b>0,347</b>	<b>0,305</b>
<b>RSD%</b>	<b>0,272</b>	<b>0,303</b>	<b>0,339</b>	<b>0,300</b>



<b>System Type</b>	X-Y-Z Robot
<b>Sample Capacity (2ml vials)</b>	160
<b>Sample Capacity (10/20 ml vials)</b>	65
<b>Solvent / Waste Vials</b>	5 / 5
<b>Minimum Sample Injection</b>	0.1 $\mu$ l
<b>Maximum Sample Injection</b>	500 $\mu$ l
<b>Syringe sizes</b>	5, 10, 25, 50, 100, 250, 500 $\mu$ l
<b>Injection per Vial</b>	up to 100
<b>Injection port</b>	up to 3
<b>Vial presence sensor</b>	YES
<b>Parameter control</b>	Pre/Post injection solvent washing, Sample/IS rinse (number/volume), Sample vial depth Syringe strokes before injection, Plunger sampling speed, Plunger injection speed, Pre/Post injection delay, Viscosity delay, Solvent plug volume, Internal standard volume, Sample volume, Air plug volume, Priority vial/sequence







## ... *on-column injection in FAST GC*

Automated **FAST ON-COLUMN** injector allows the injection of nano to macro volume of liquid sample directly into narrow and ultra narrow (50-250 microns) capillary columns.


- True cold on-column injection in FastGC
- No sample dilution
- No use of pre-column
- Fully automatic

## ... *takes advantage of*



- No discrimination effect on wide range boiling points
- No sample degradation of thermally-labile compounds
- No impurities from septa
- Wide range of injection volume (from nanoliters to microliters)

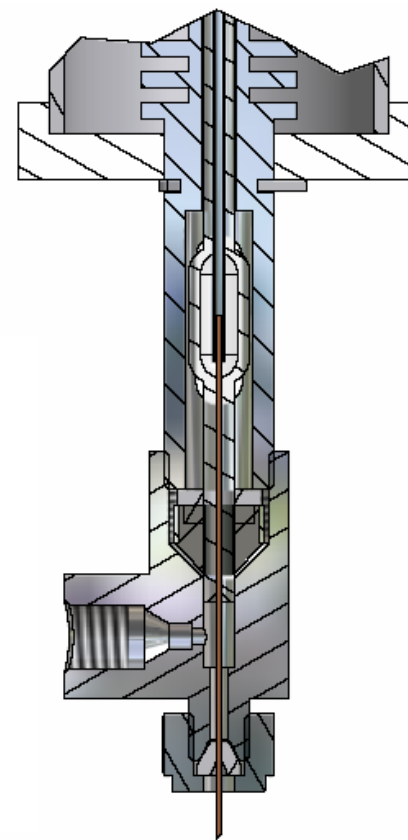


## *Principle of operation*

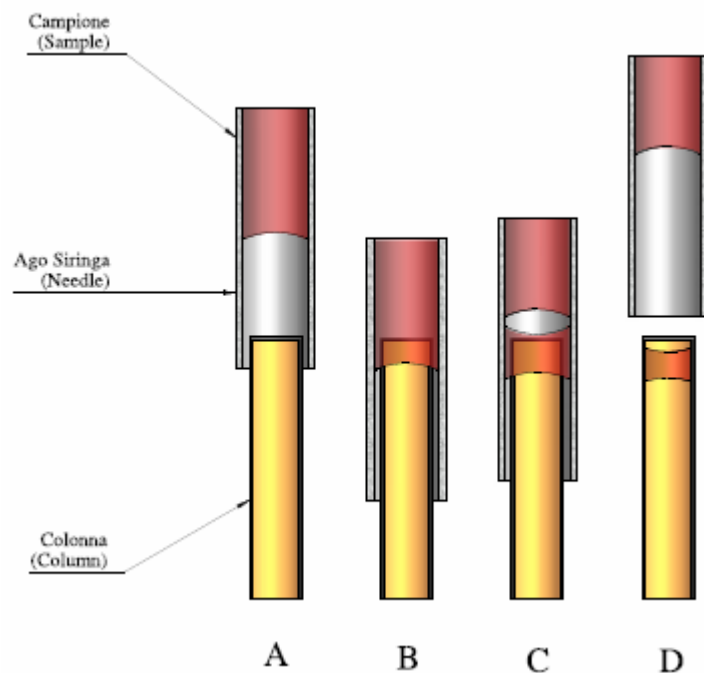

- A) The syringe needle slides over the capillary column**
- B) The column comes in contact with the liquid**
- C) The liquid is sampled by capillarity**
- D) The needle withdraws and the analysis starts**




# *Automated Fast On-column*

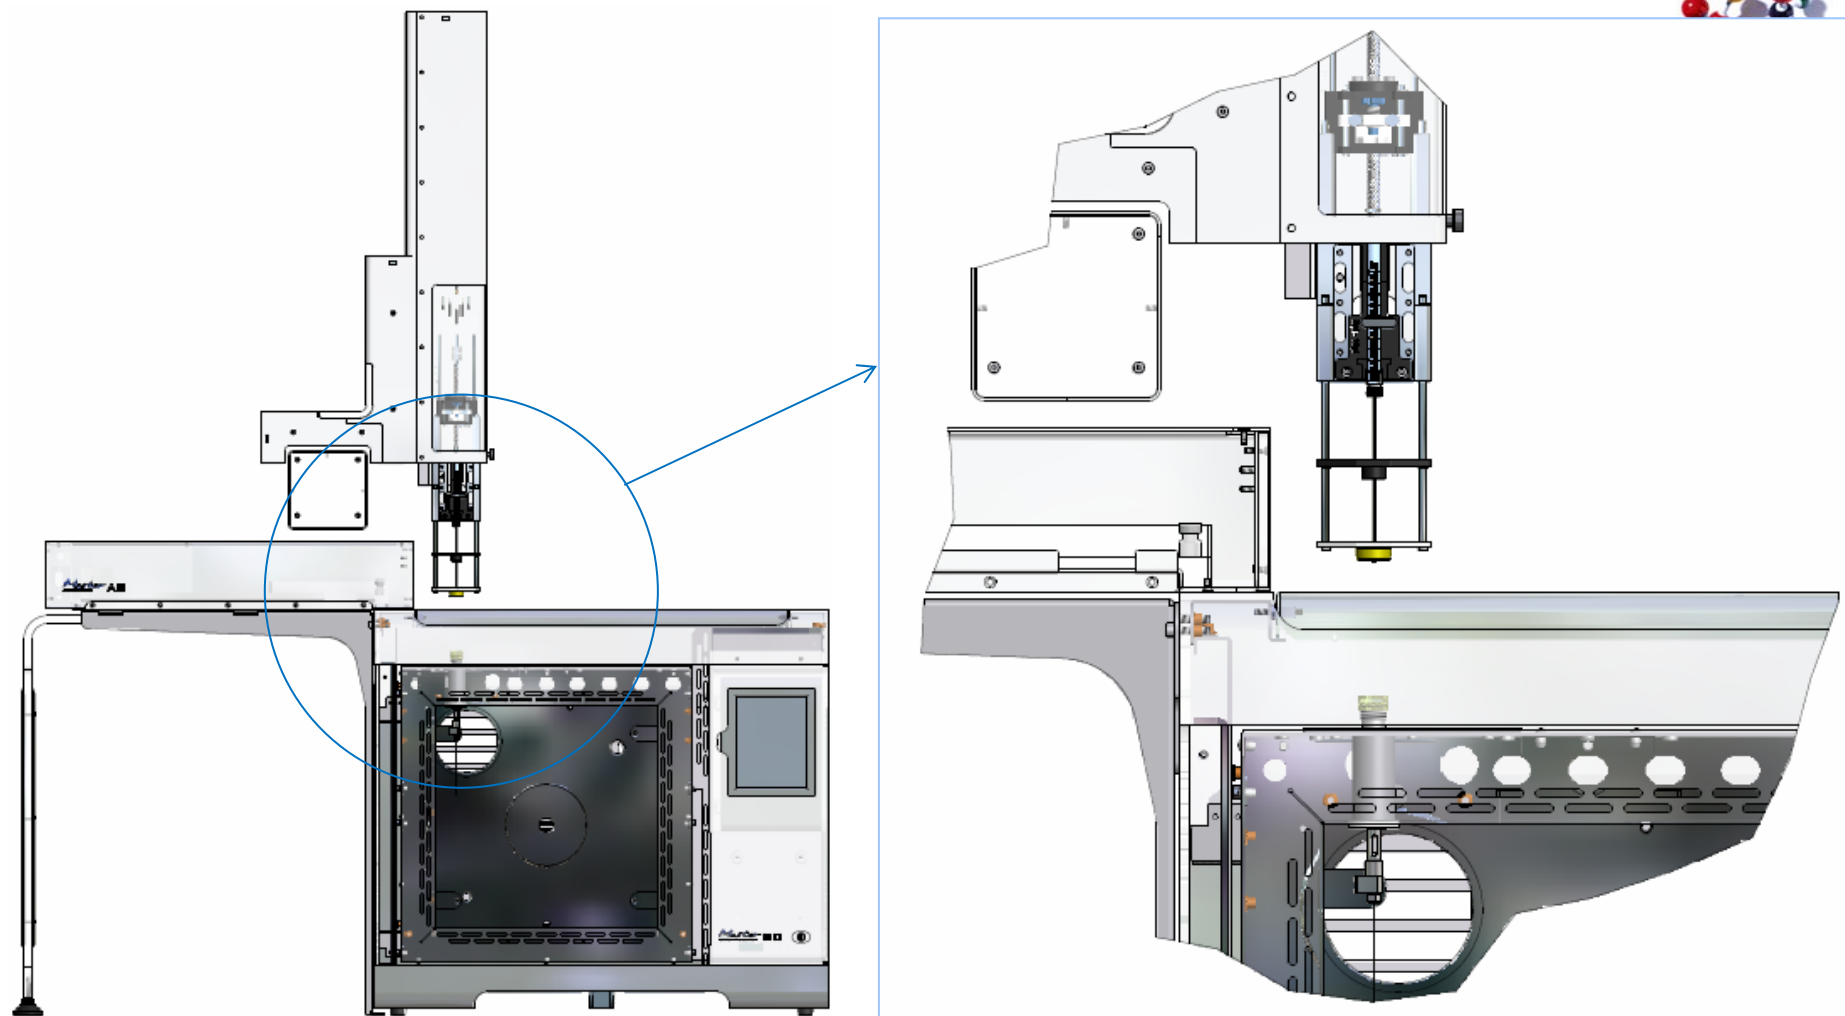

Automated FAST ON-COLUMN

# SAGE Essential Oil FAST-GC

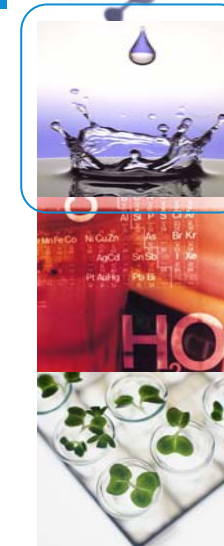

Hot Injection

FAST ON-COLUMN\*


**Split Ratio  
1:1000**

Injector and  
needle  
discrimination

Sample  
Alteration

Non diluted  
Sample

**10  
nL**

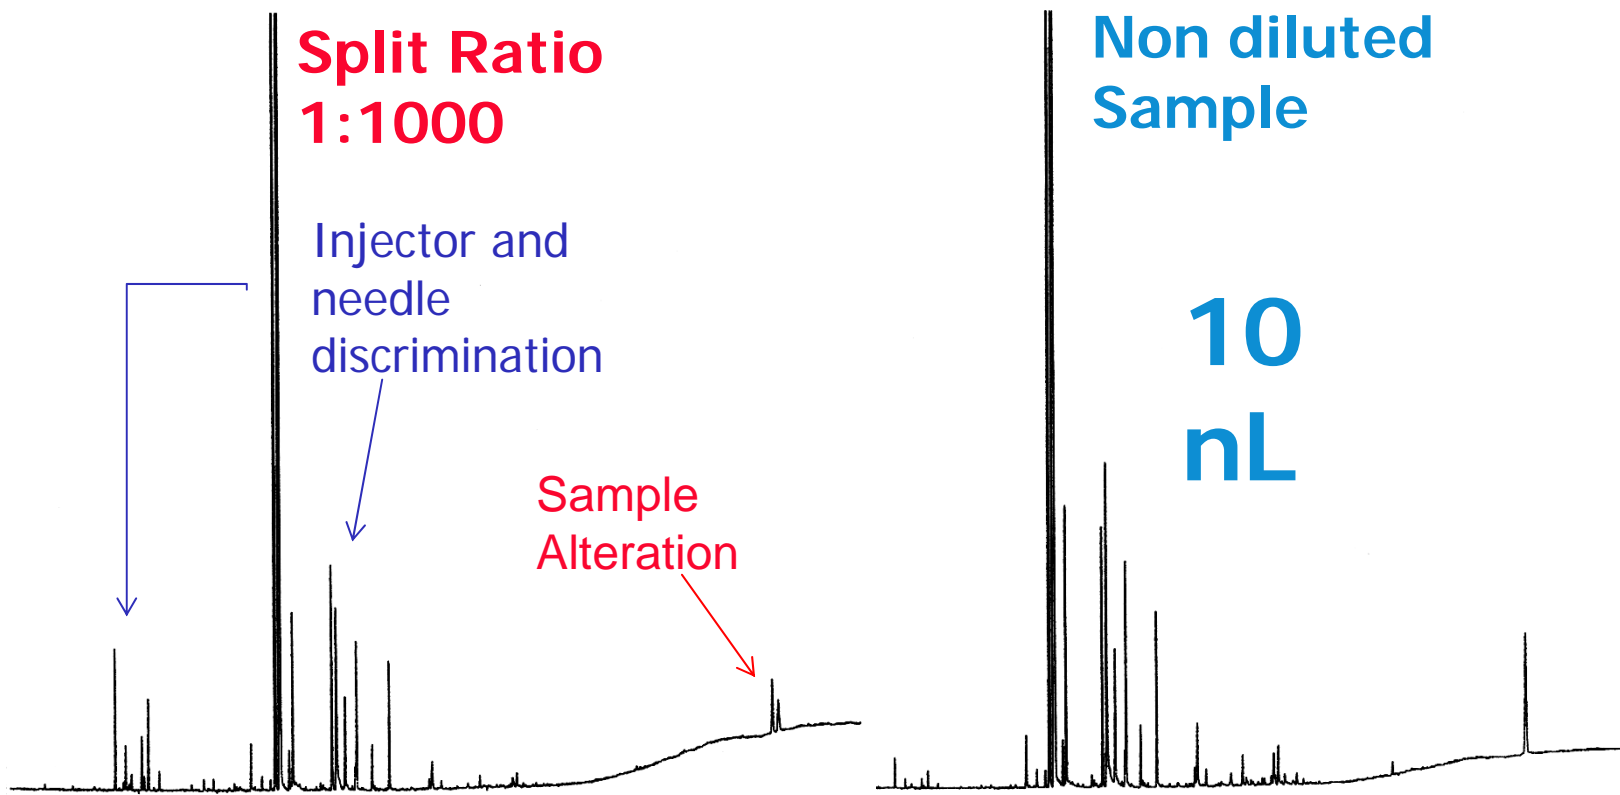

Column: 10 m L x 100 µm i.d., 0.1 µm f.t. DN-WAX  
Oven: 40°C – 15°C/min – 230°C  
Carrier gas: Hydrogen at 59 cm/s



**10 min  
analysis time**

\* Patent Pending System

Automated FAST ON-COLUMN



## Automated Fast On-column Performances

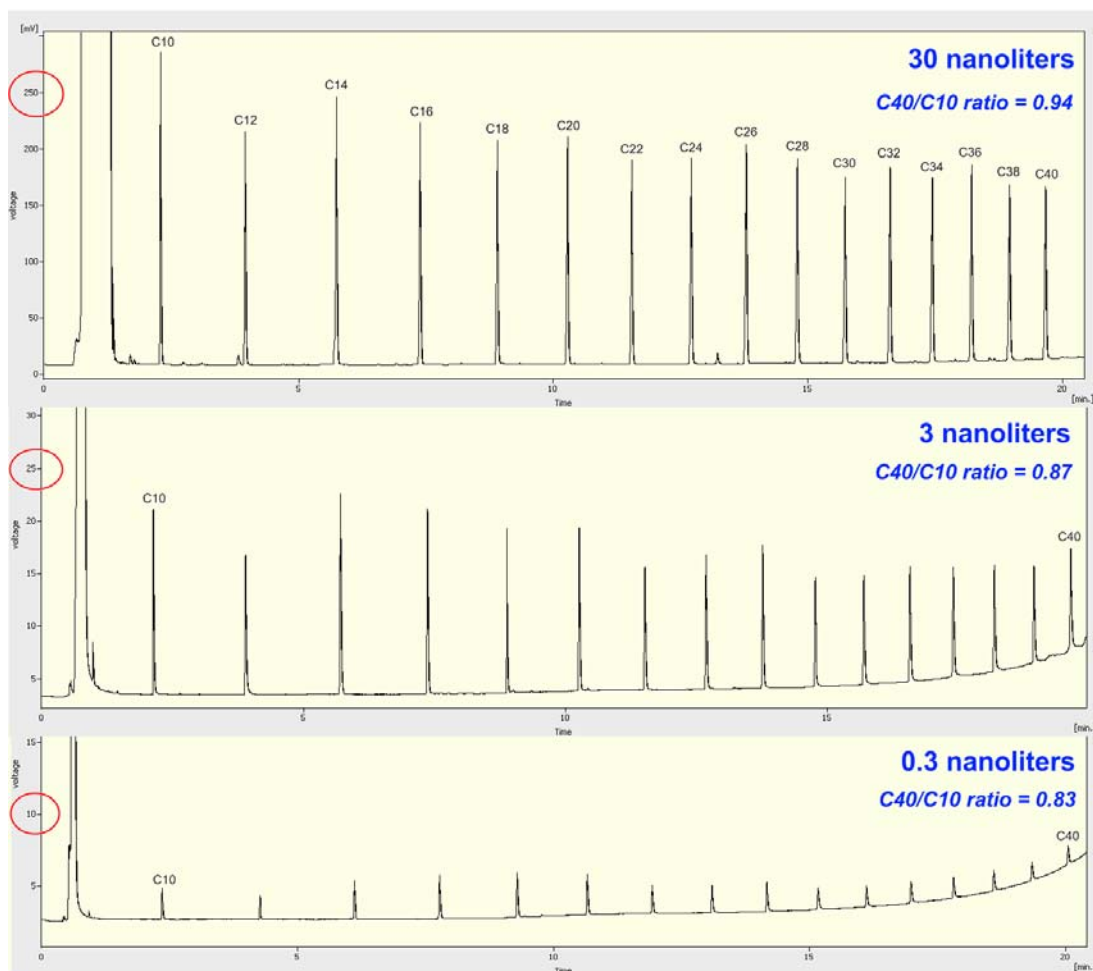

This application shows the performances of the FAST On-Column Inlet system (\*) with an introduction of Alkane Mixture from 30nL down to 0.3nL direct liquid injection into the column! The discrimination is minimized like a traditional On-Column injection.

FLUKA Cat.# 68281, "Alkane Standard Mixture for the assay of the system efficiency of GC's C10-C40"

**Column:**

5 m L x 250  $\mu$ m i.d., 0.1  $\mu$ m f.t. DN-1


**Oven:**

40°C – 15°C/min – 350°C

**Carrier gas:**



Helium at 30 kPa

# Butter TRIGLYCERIDES FAST-GC

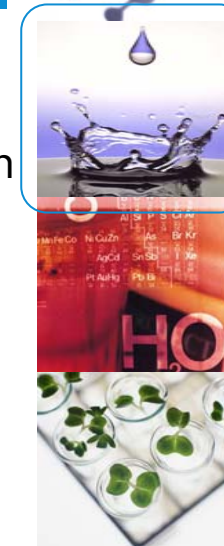

Hot Injection

FAST ON-COLUMN\*


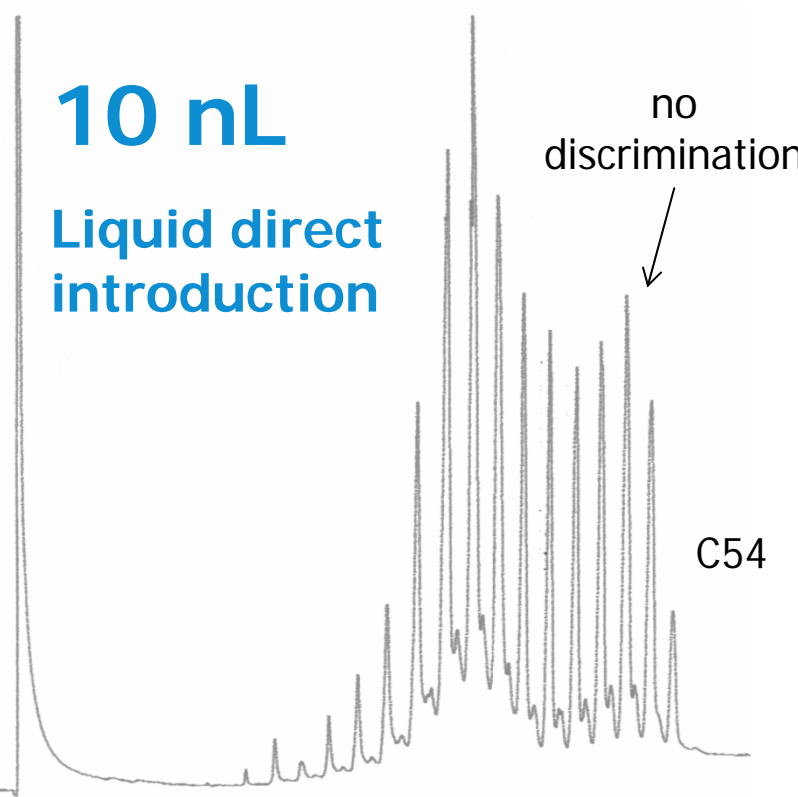
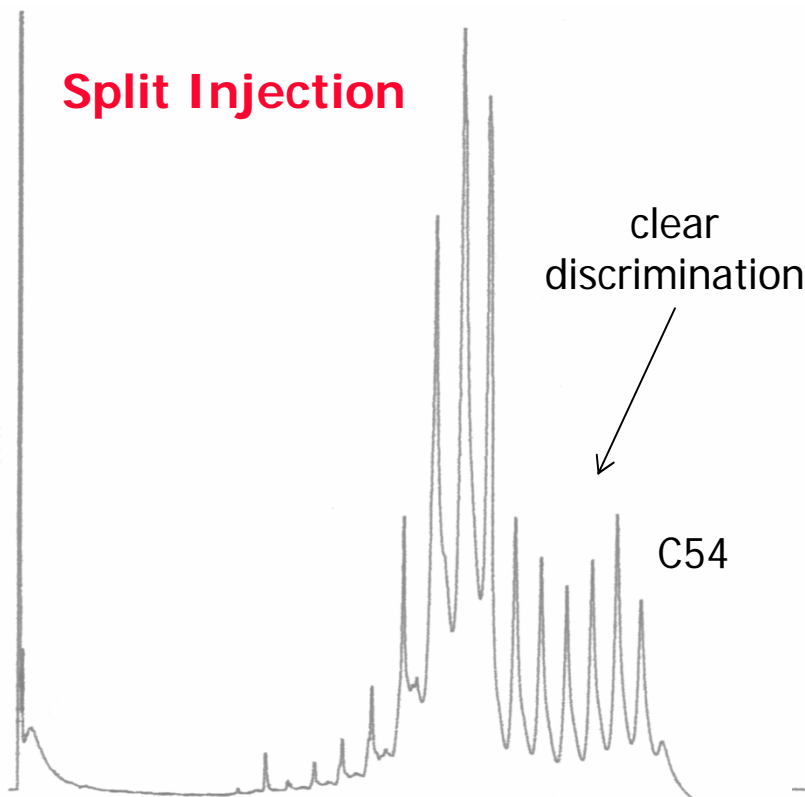


**Column:** 1.5 m L x 100  $\mu$ m i.d., 0.1  $\mu$ m f.t. DN-1  
**Oven:** 100°C – 30°C/min – 350°C  
**Carrier gas:** Hydrogen at 150 kPa

**8 min  
analysis time**

\* Patent Pending System

Automated FAST ON-COLUMN



## MASTER TOF – Time of Flight GC-MS

## *Master TOF* Time of Flight Mass Spectrometer

### *... the true Fast GC-MS*




- only Time of Flight Mass Spectrometer offers the required performance for the acquisition of very fast peak
- MasterTOF Time of Flight MS has been especially designed for Fast GC and GCxGC applications.
- With an acquisition rate up to 500 spectras/s, **MASTER TOF** guarantees a proper peak **identification** and **quantitation** also in complex matrices

### *... wide linearity*


- a wide dynamic range ( $10^5$ ) **decreases** the need of dilution of highly concentrated sample, increasing the throughput of the laboratory

### *... powerful Deconvolution Software*




- mass spectra automatically extracted free of interferences from system, matrix background and coeluting analytes
- analyte identification by spectral identification or by library search using **NIST library** or operator-prepared databases.




*Master TOF*  
Time of Flight Mass Spectrometer

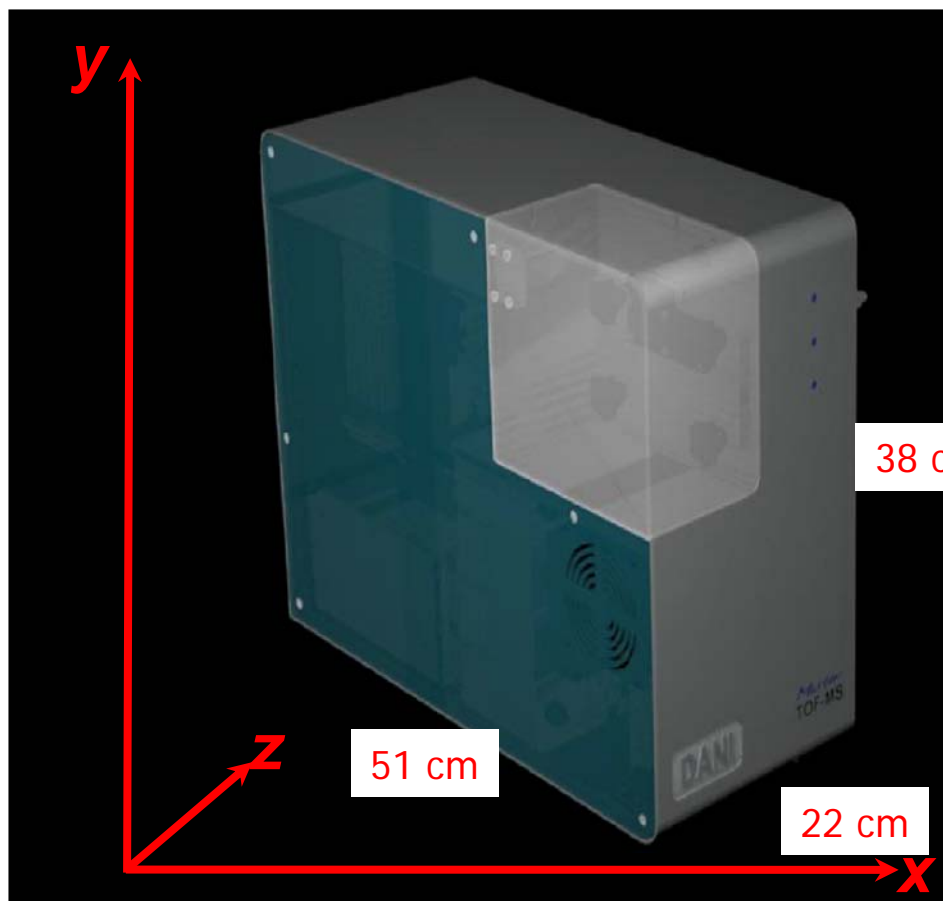

Extremely compact design for bench top space saving





## *Master TOF* Time of Flight Mass Spectrometer

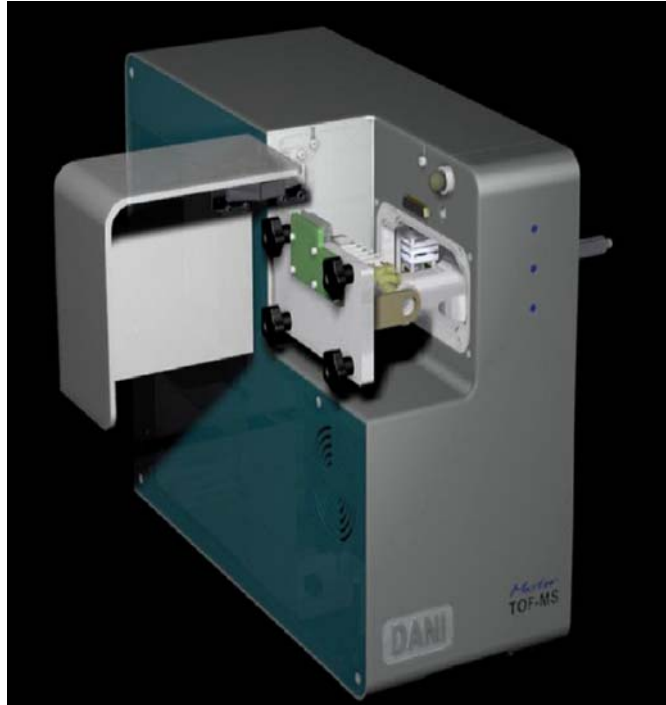

Extremely easy access to the ion source and flight chamber for an effective, complete cleaning and replacement of all the components

- Fast and efficient maintenance procedure
- No special tools needed

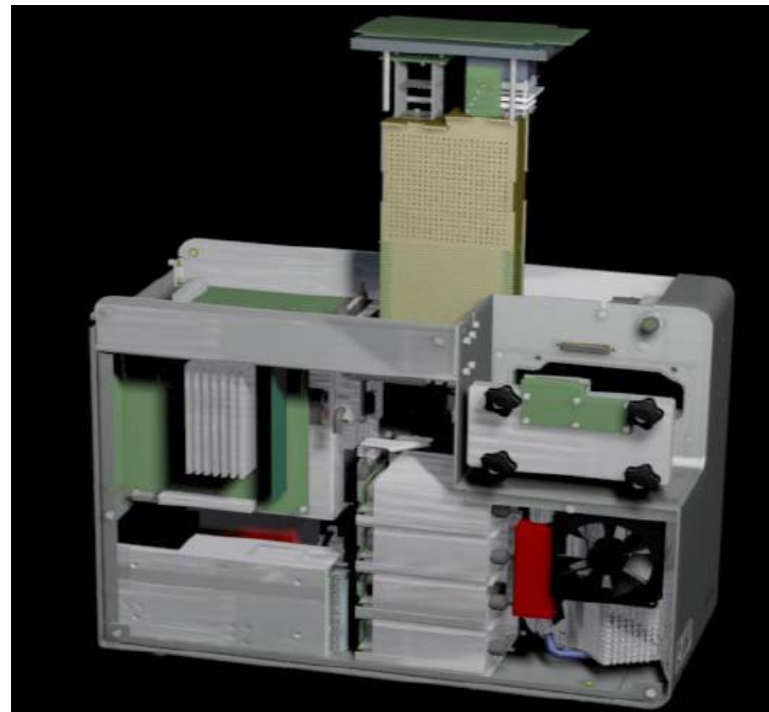

## *Master TOF*




### Time of Flight Mass Spectrometer

#### DANI Master TOF Acquisition Numbers

- Acceleration field pulsed at 30 KHz
- This generates 30,000 spectra/s
- The system averages the spectra to “only” 500 centroid spectra/s to disk, to ensure more feasible transfer rates and more representative spectra
- 1000 spectra/s are possible under extreme conditions

#### DANI Master TOF Software Package




- Master AS/GC software control included
- Peak assignment based on automatic deconvolution procedure
- Library search with NIST MS Search



# Master TOF Time of Flight Mass Spectrometer


## Specifications

<b>Mass Range</b>	5 to 1500 amu
<b>Acquisition rate</b>	Up to 1000 spectra/s
<b>Sensitivity</b>	1 pg Octafluoronaphthalene s/n > 10:1 at m/z 272
<b>Resolution</b>	1500
<b>Linearity</b>	10 <sup>5</sup>
<b>Tune mode</b>	Automatic Full Autotune Automatic Autotune Manual Tune
<b>Ion Source</b>	EI – Standard CI (+/-) Optional
<b>Vacuum System</b>	Internal Diaphragm Pump 2 Turbomolecular pumps 260-70 L/s

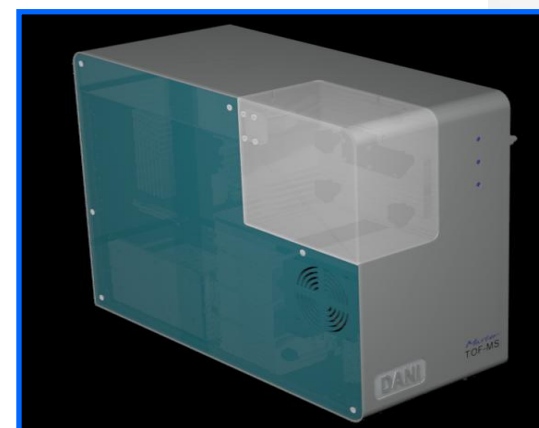





## Sensitivity


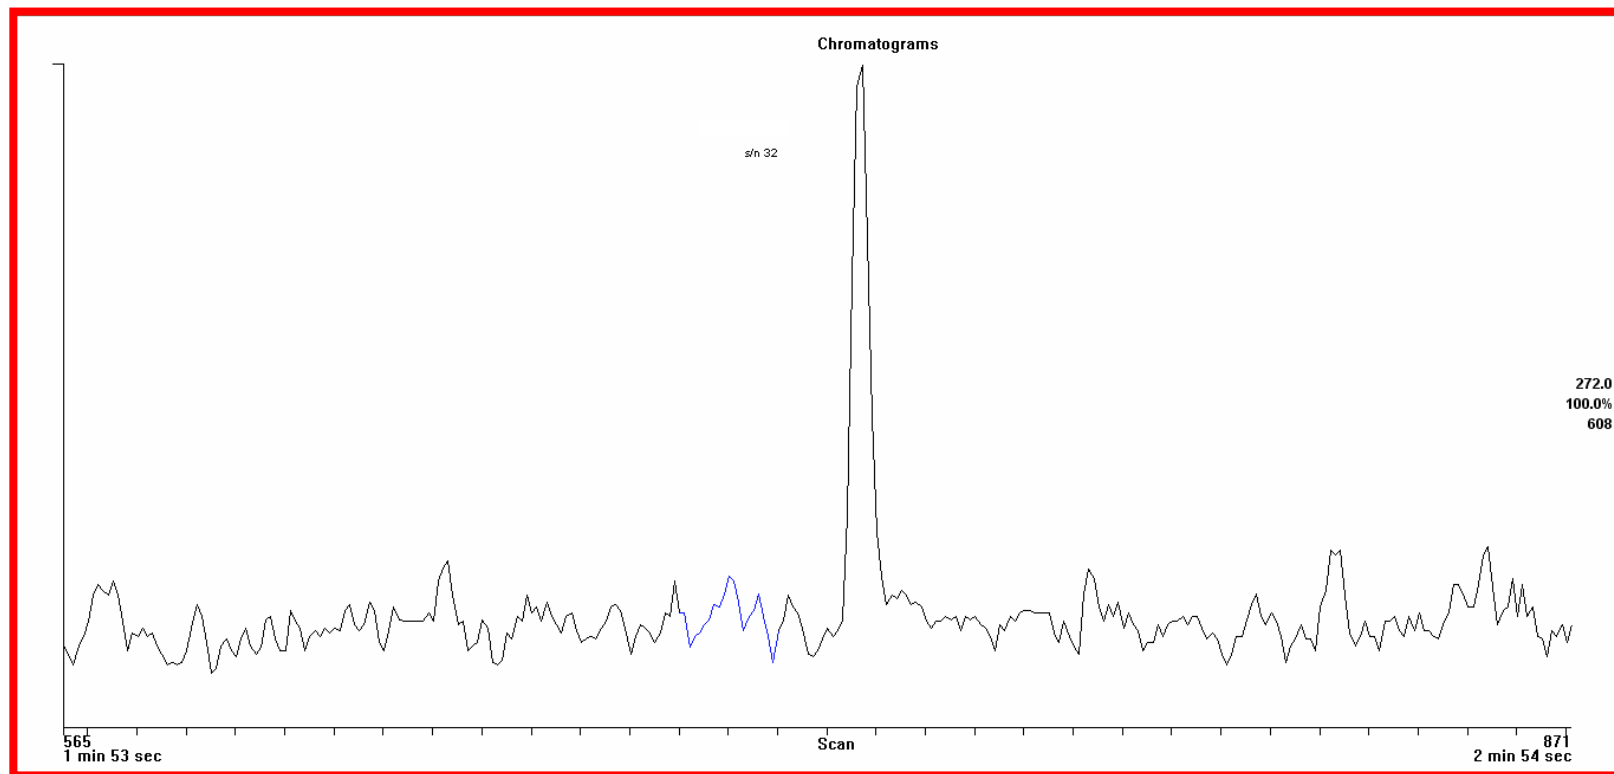


1 pg OFN (Octafluoronaphthalene)




# Master TOF Time of Flight Mass Spectrometer

## FAST GC ANALYSIS OF CITRUS ESSENTIAL OILS



**LEMON OIL**

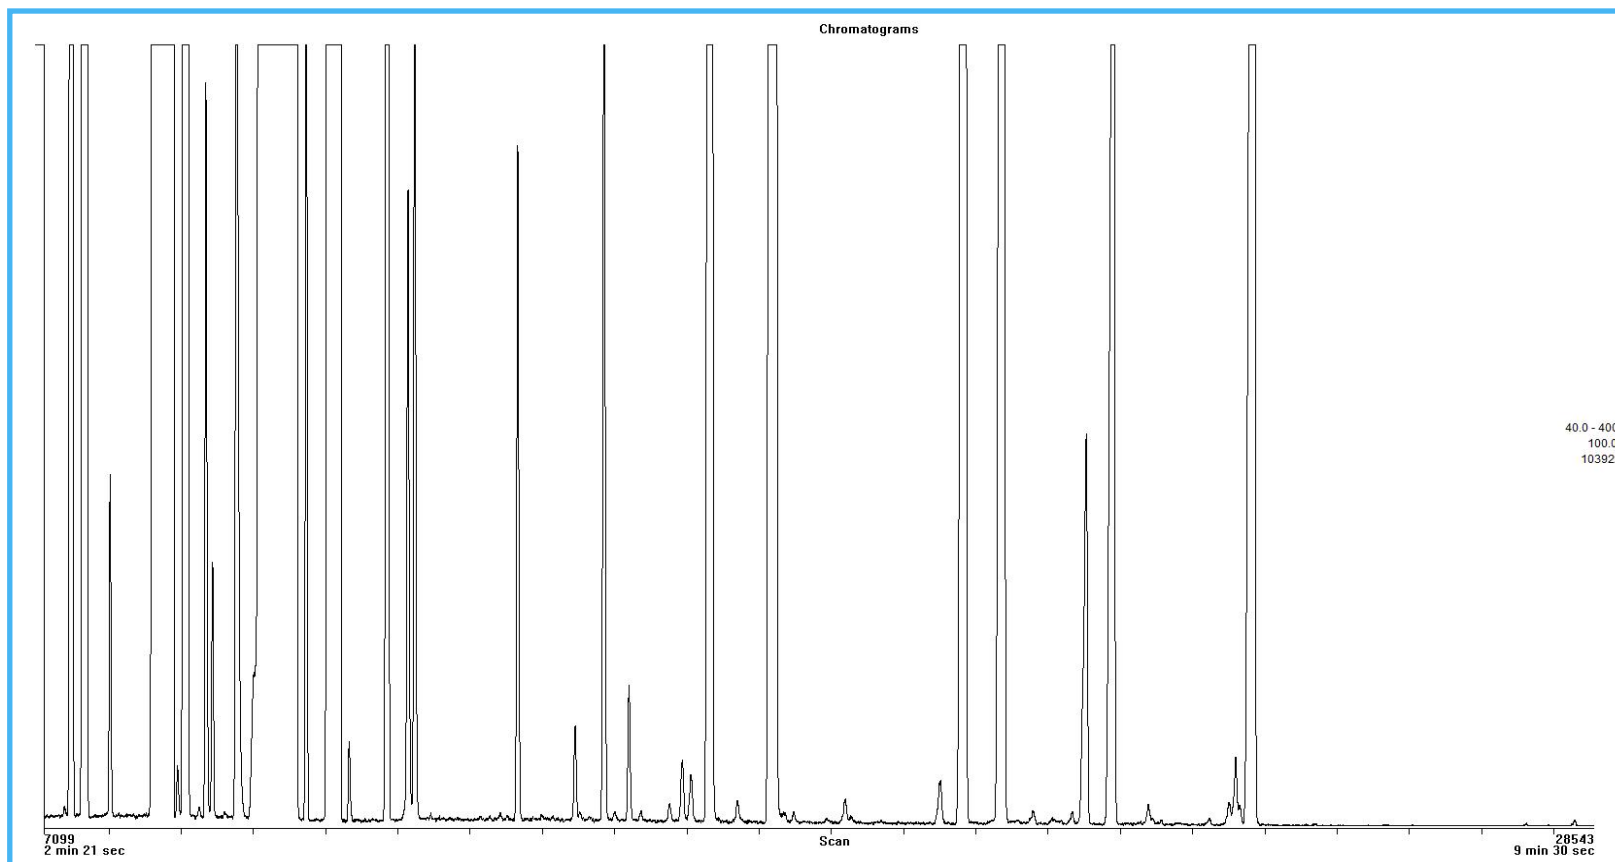

Sample: Lemon oil 1:100 in Heptane




### Gas Chromatograph Method

Injector: Split-Splitless, Injector Temperature: 250°C, Injector Volume: 1.0  $\mu$ l, Split Ratio: 1:20, Column: DN-5 10 m x 0.1 mm x 0.1  $\mu$ m

Linear Velocity: 40 cm/sec at constant linear velocity, Oven Temperature Program: from 50°C to 250°C (0.72 min) at 14°C/min

### Time of Flight

Transfer line temperature: 220°C, Sampling rate: 50 Hz, Mass range: 40-400 amu, Solvent delay: 120 sec, Acquisition time: 10 min

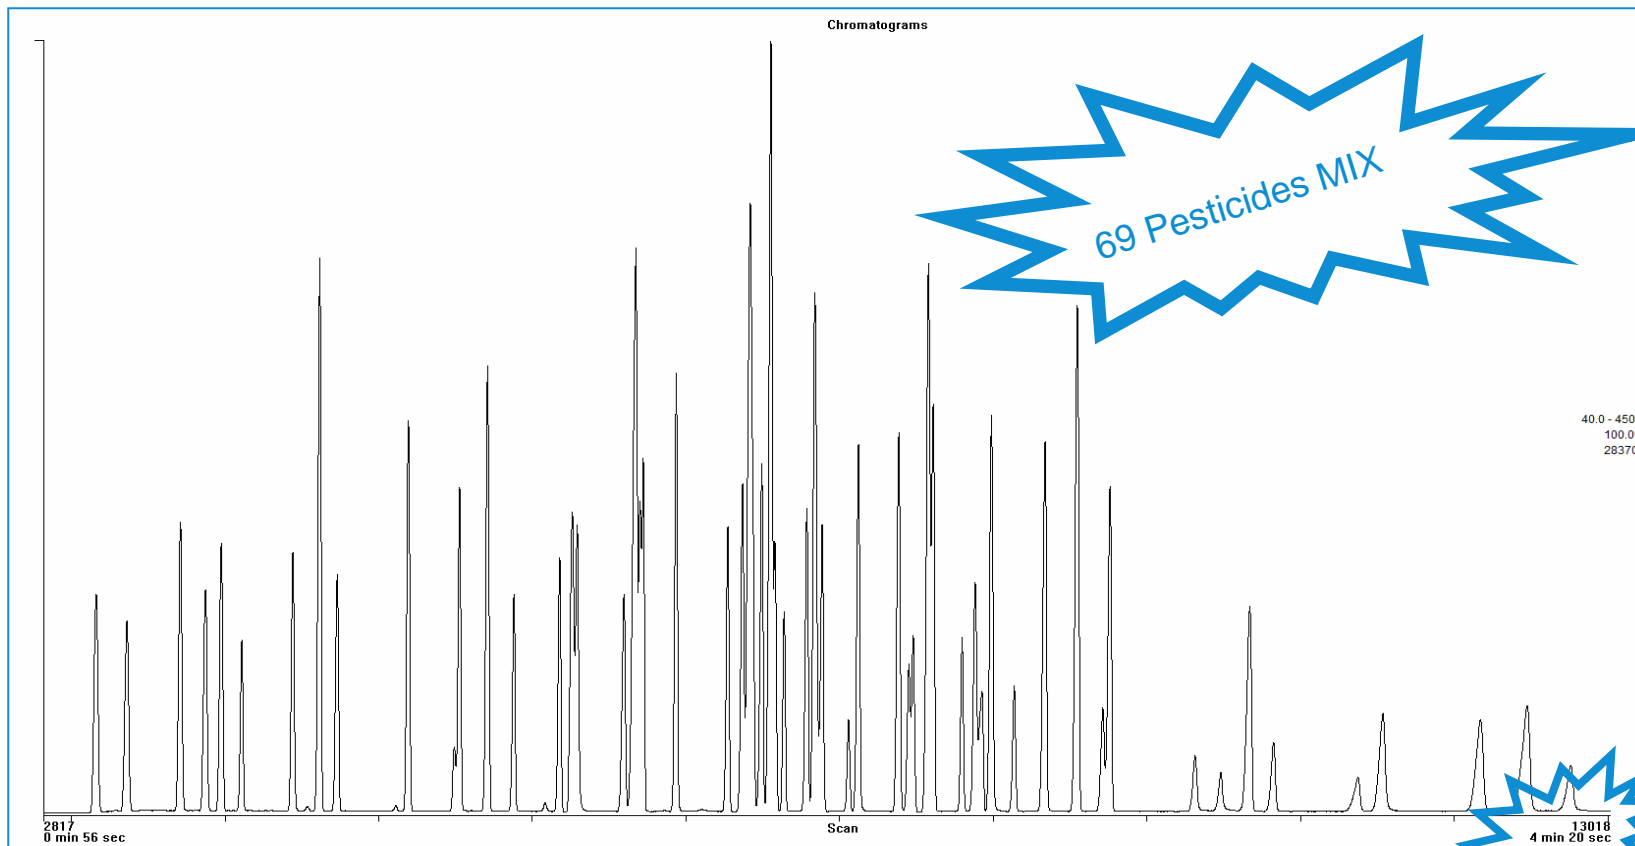

Sample: Pesticides Mix, Solvent and concentration: 100 ppm in Acetone

### Gas Chromatograph Method

Injector: Split-Splitless, Injector Temperature: 250°C, Injector Volume: 1.0  $\mu$ l, Split Ratio: 1:50, Column: DN-1701 10 m x 0.1 mm x 0.1  $\mu$ m

Column Flow: 0.5 ml/min at constant flow, Oven Temperature Program: from 100°C to 280°C (for 1.5 min) at 50°C/min




### Time of Flight

Transfer line temperature: 220°C

Sampling rate: 100 Hz, Mass range: 40-450 amu, Solvent delay: 60 sec, Acquisition time: 4.5 min

# Master TOF Time of Flight Mass Spectrometer

## FAST GC ANALYSIS OF PESTICIDES AUTOMATIC SOFTWARE DECONVOLUTION

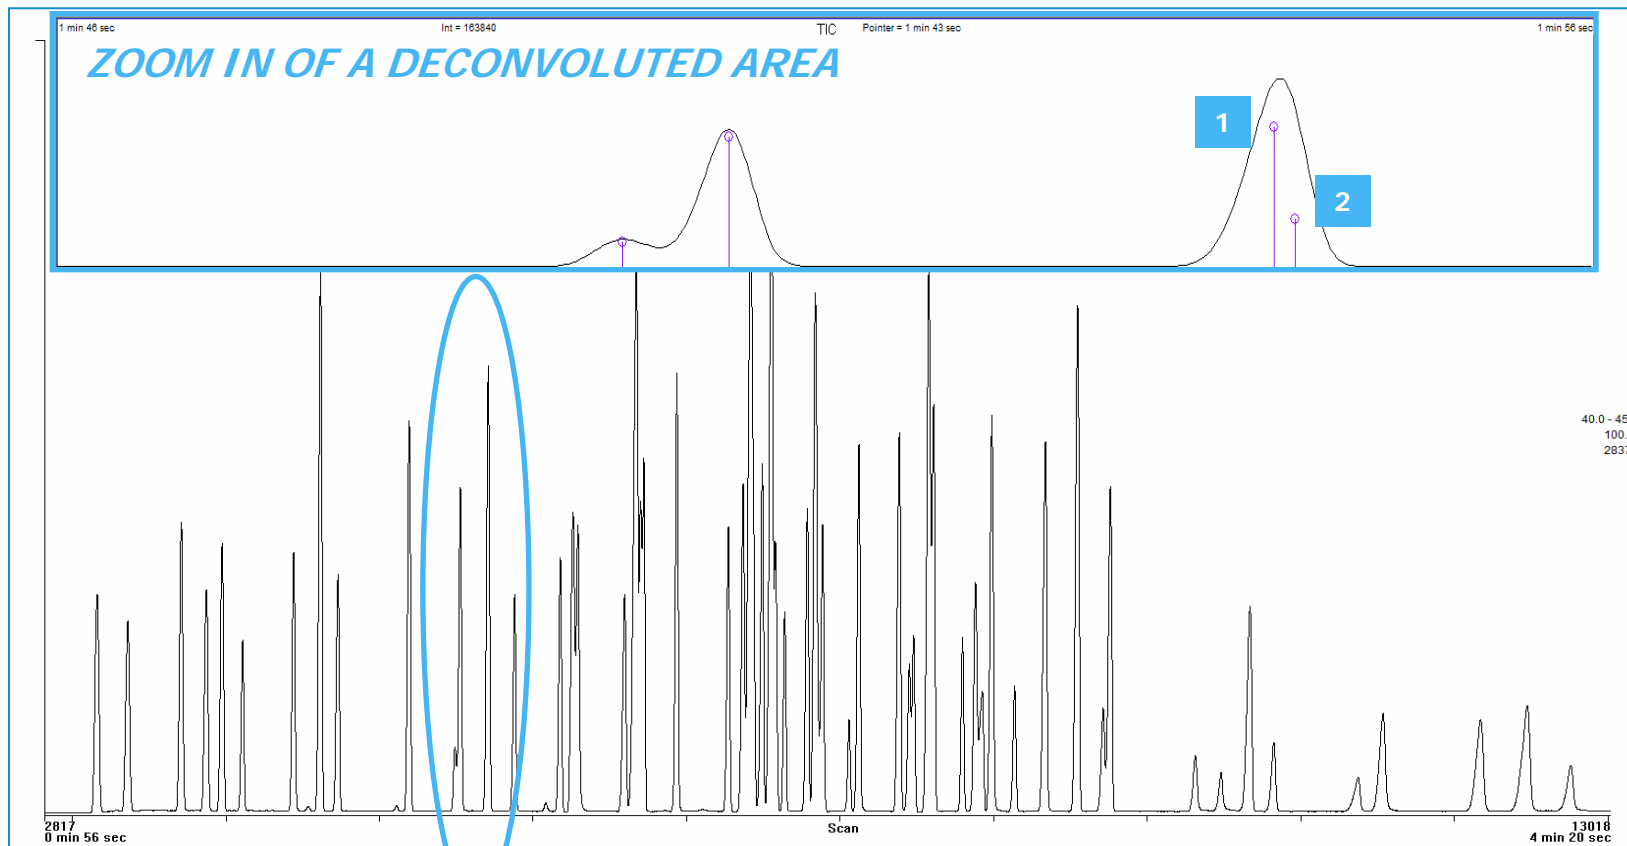

Sample: Pesticides Mix, Solvent and concentration: 100 ppm in Acetone

### Gas Chromatograph Method

Injector: Split-Splitless, Injector Temperature: 250°C, Injector Volume: 1.0  $\mu$ l, Split Ratio: 1:50, Column: DN-1701 10 m x 0.1 mm x 0.1  $\mu$ m

Column Flow: 0.5 ml/min at constant flow, Oven Temperature Program: from 100°C to 280°C (for 1.5 min) at 50°C/min





### Time of Flight

Transfer line temperature: 220°C

Sampling rate: 100 Hz, Mass range: 40-450 amu, Solvent delay: 60 sec, Acquisition time: 4.5 min




# Master TOF Time of Flight Mass Spectrometer

## FAST GC ANALYSIS OF PESTICIDES LIBRARY SEARCH RESULTS

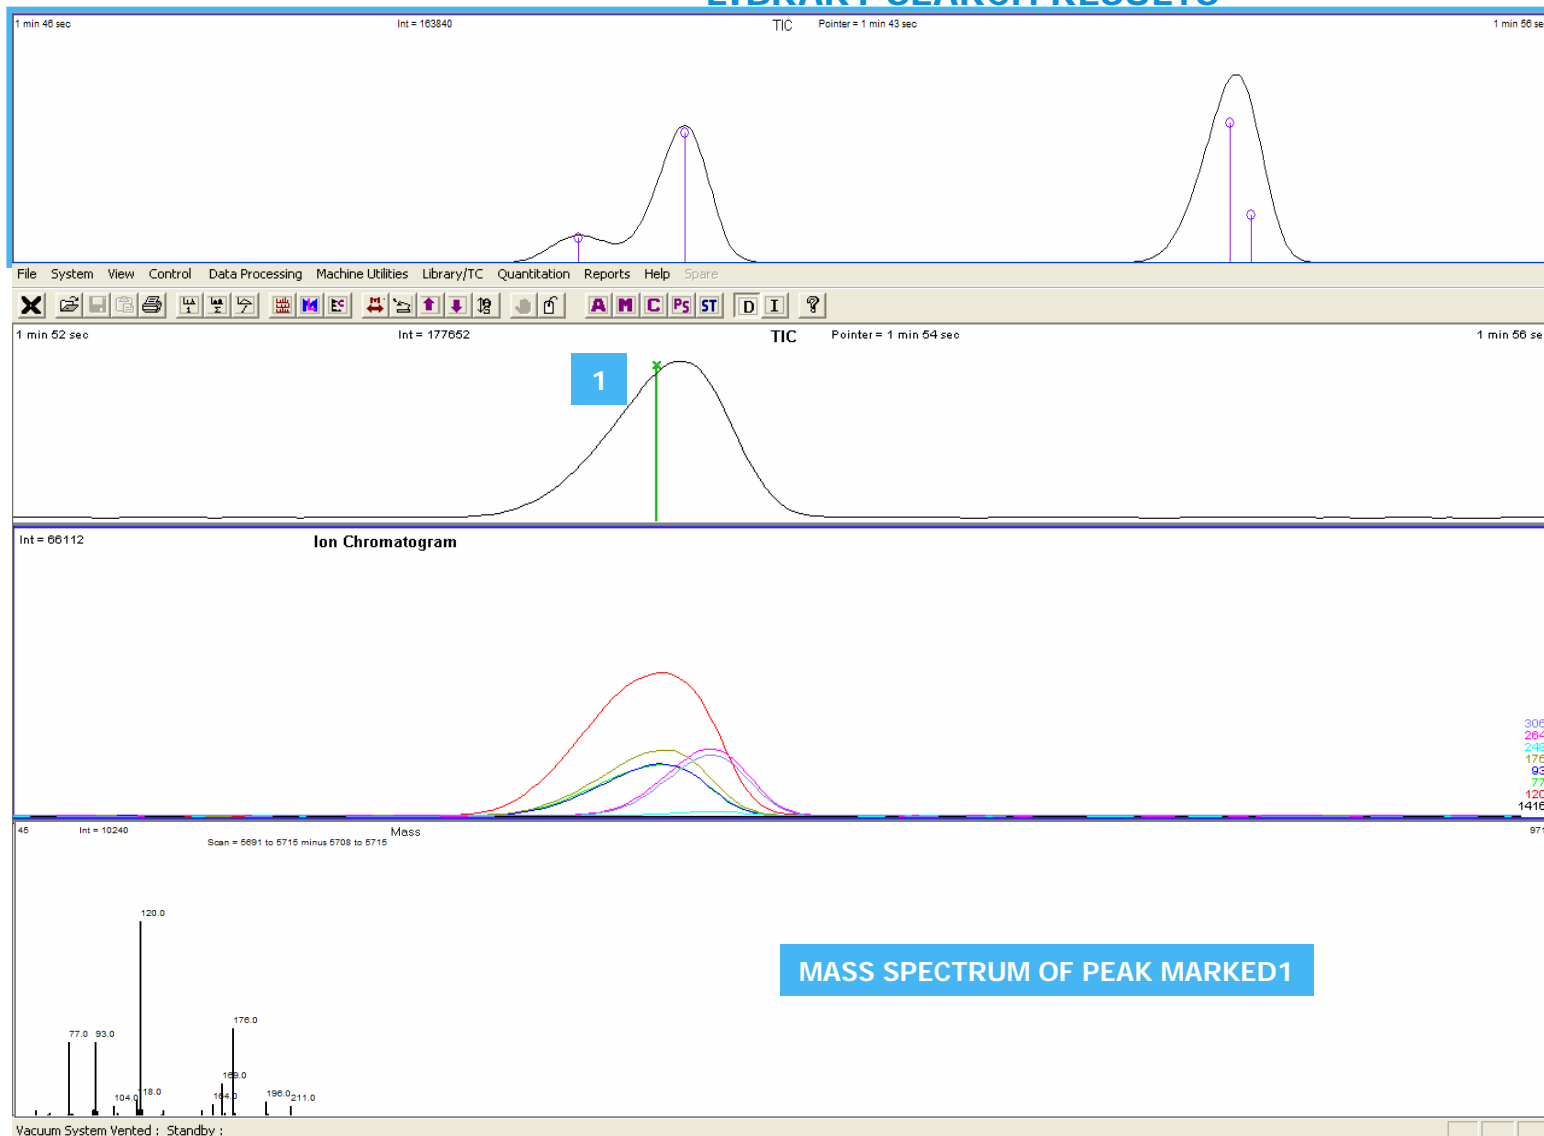



# Master TOF Time of Flight Mass Spectrometer

## FAST GC ANALYSIS OF PESTICIDES LIBRARY SEARCH RESULTS

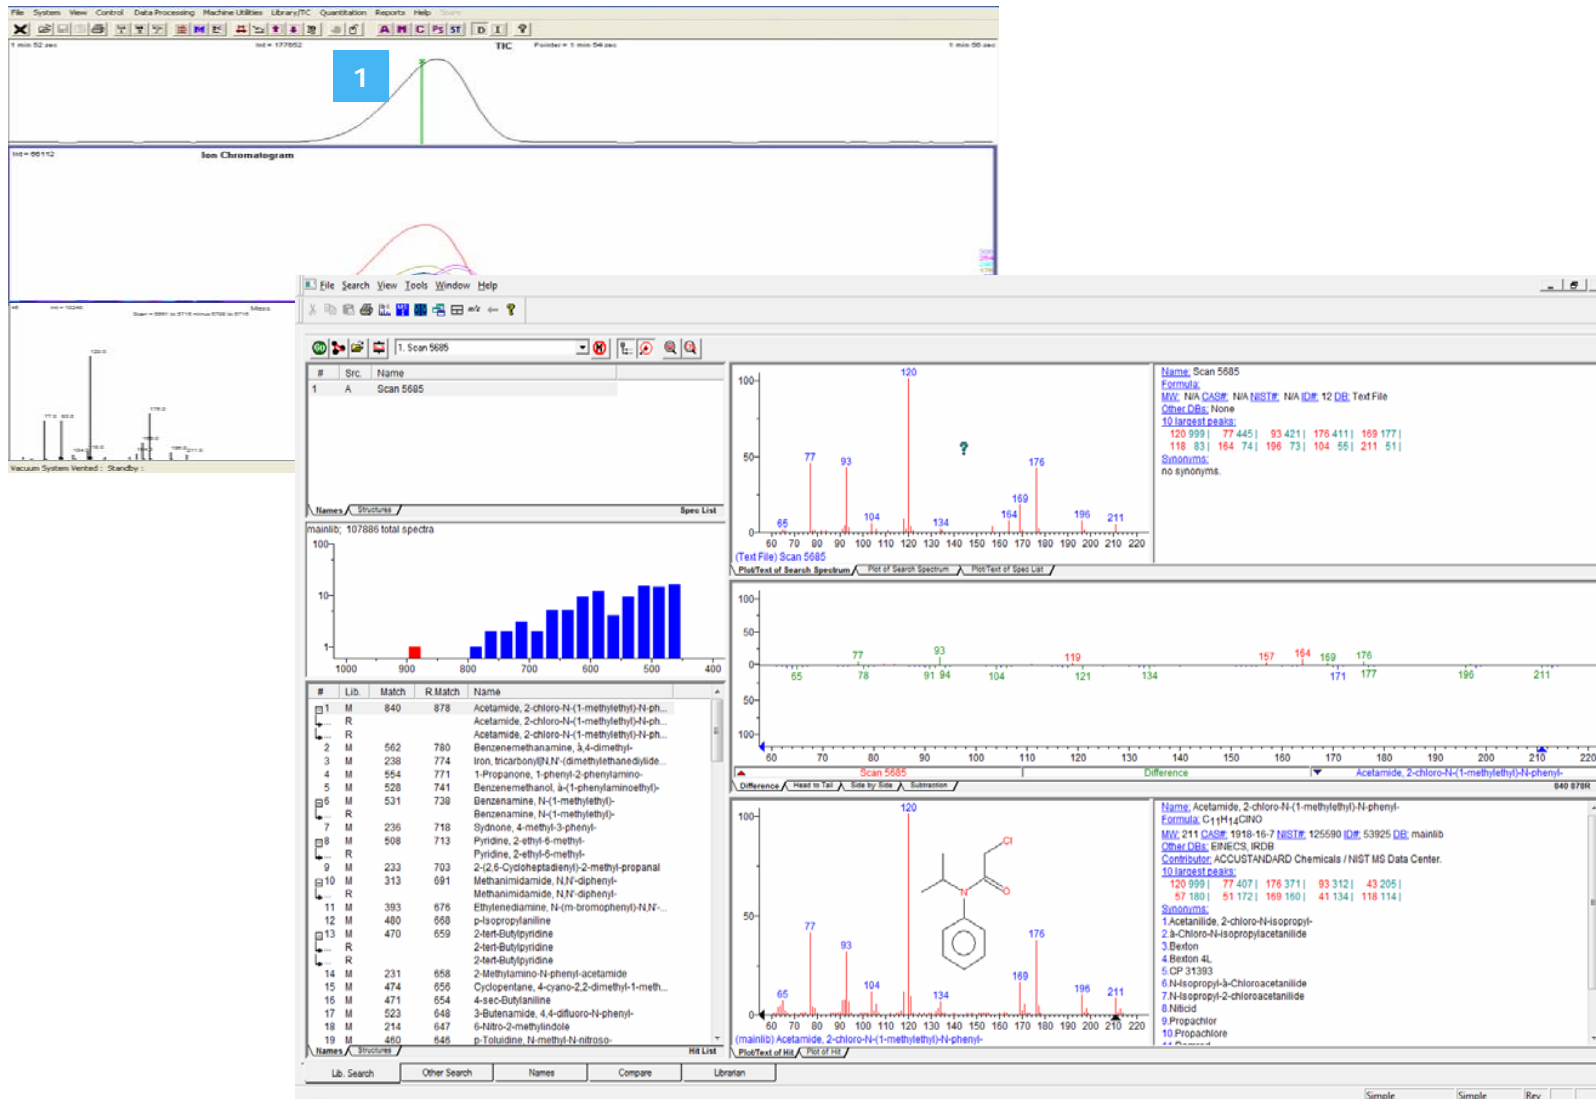
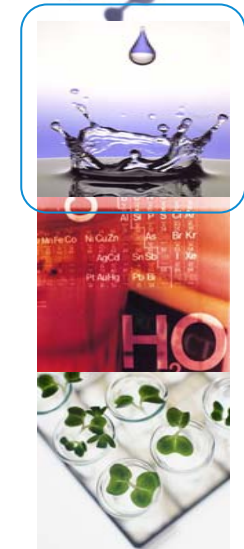



# Master TOF Time of Flight Mass Spectrometer

## FAST GC ANALYSIS OF PESTICIDES LIBRARY SEARCH RESULTS




## FAST GC ANALYSIS OF PESTICIDES LIBRARY SEARCH RESULTS





## Pesticides Determination in Essential Oil


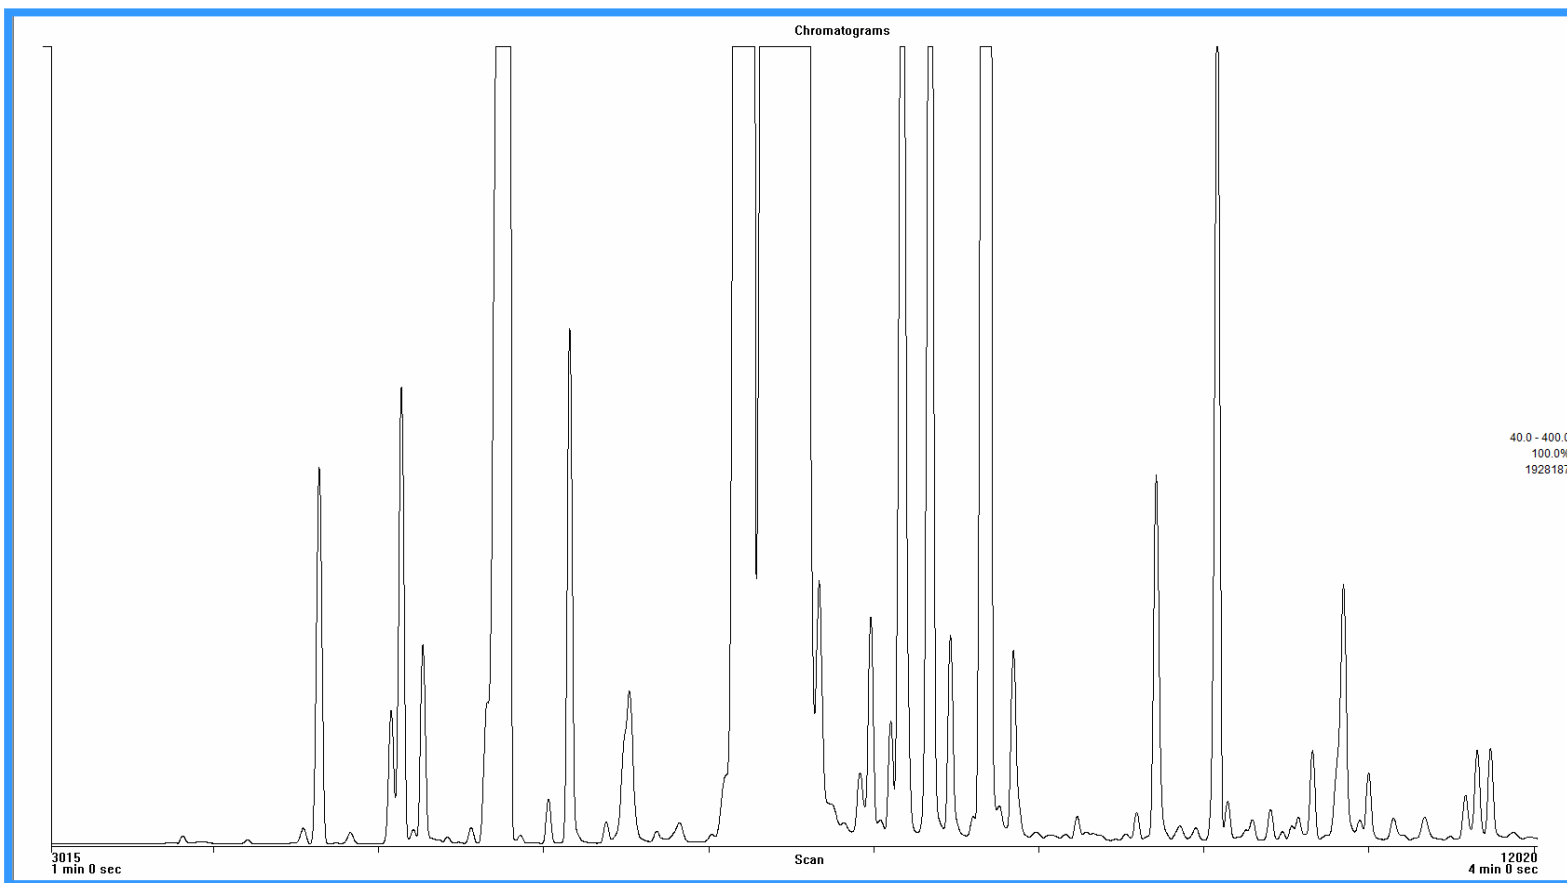


### Gas Chromatograph


Injector: Split-Splitless  
Injector Temperature: 250°C  
Injector Volume: 0.5 µl  
Split Ratio: 1:10  
Column: DN-5 10 m x 0.1 mm, 0.1 µm  
Linear Velocity: 40 cm/sec at constant linear velocity  
Oven Temperature Program: from 50°C to 250°C at 40°C/min

### Time of Flight


Transfer line temperature: 220°C  
Sampling rate: 50 Hz  
Mass range: 40-400 amu  
Solvent delay: 60 sec  
Acquisition time: 5 min




Mint Oil

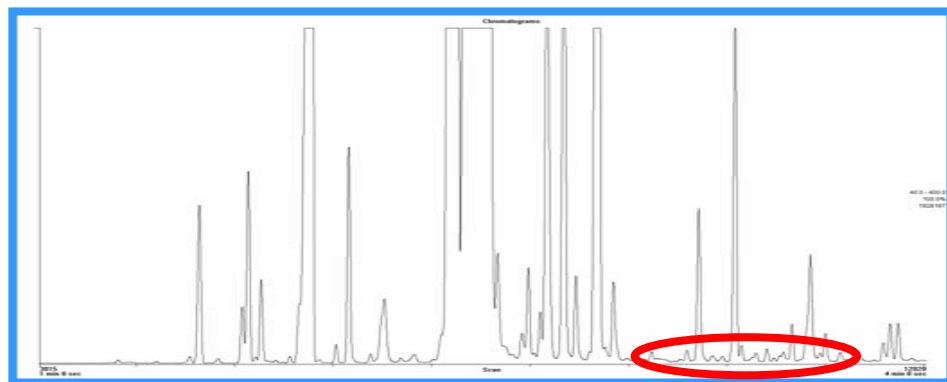



Mint oil total ion chromatogram (TIC)

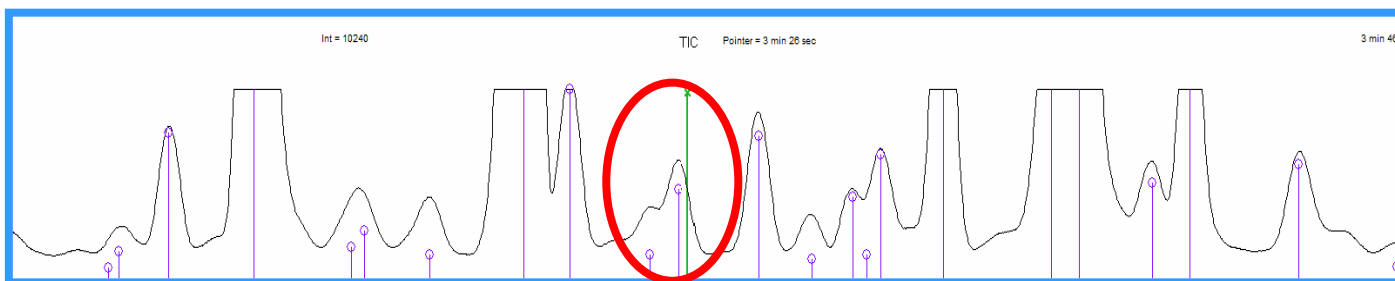




Peaks automatically software deconvoluted



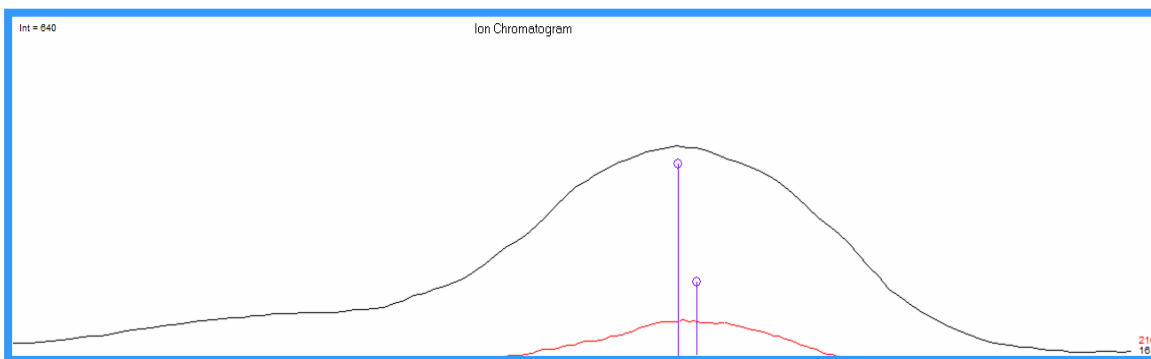


Etridiazole automatically deconvoluted



Mint Oil

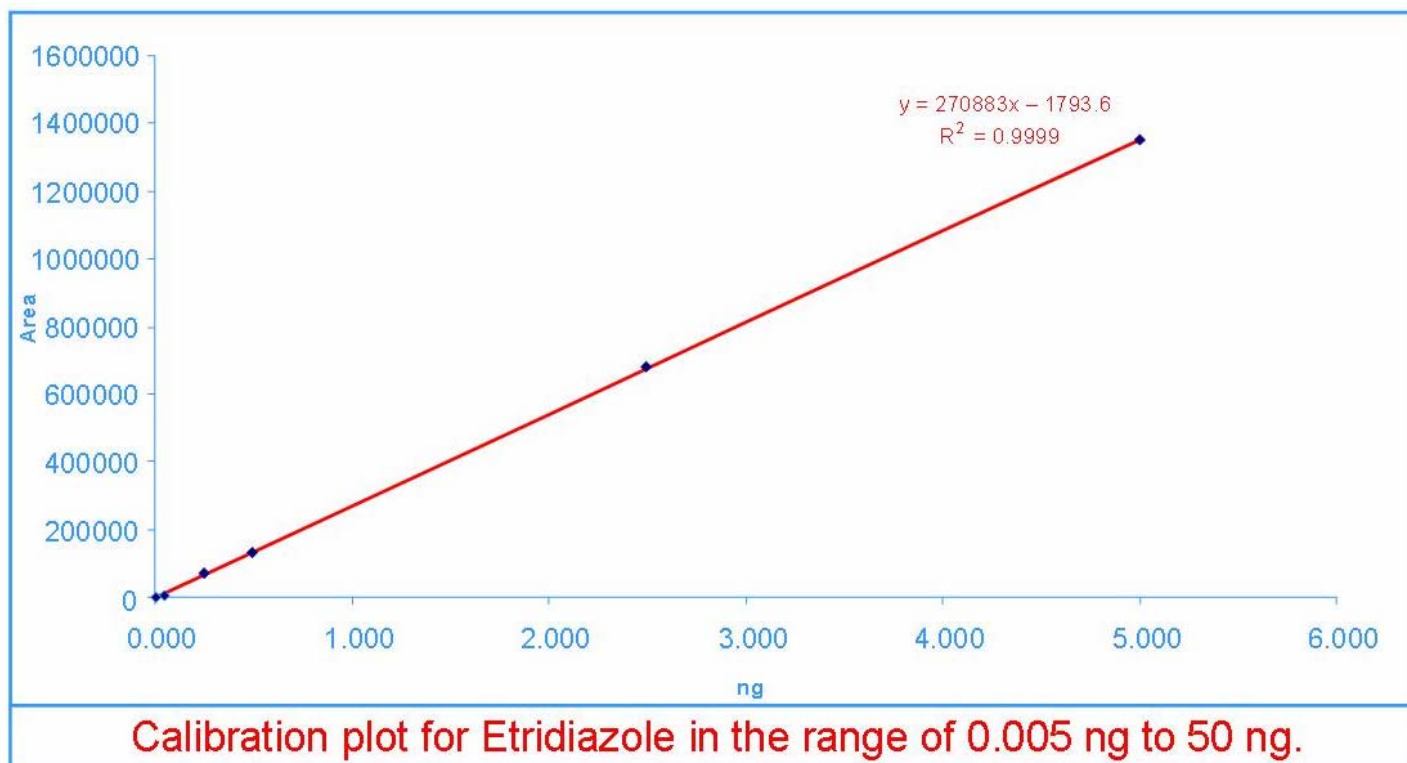

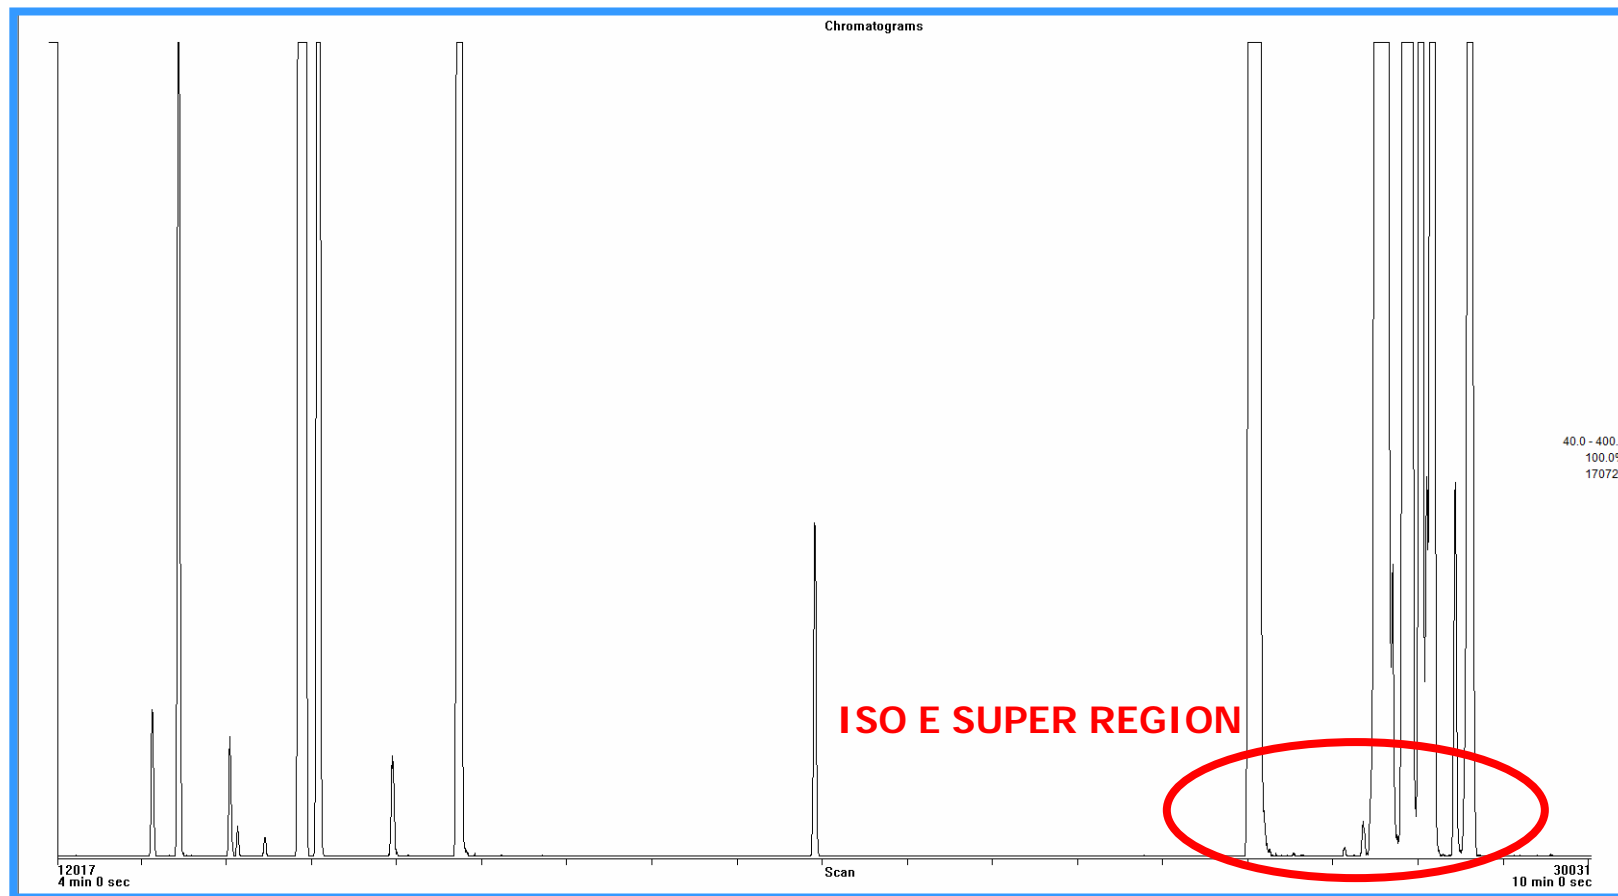


### Gas Chromatograph

Injector: Split-Splitless  
Injector Temperature: 250°C  
Injector Volume: 0.5  $\mu$ l  
Split Ratio: 1:400  
Column: DN-5 10 m x 0.1 mm, 0.1  $\mu$ m  
Linear Velocity: 40 cm/sec at constant linear velocity  
Oven Temperature Program: from 50°C to 250°C at 14°C/min

### Time of Flight




Transfer line temperature: 220°C  
Sampling rate: 50 Hz  
Mass range: 40-400 amu  
Solvent delay: 60 sec  
Acquisition time: 14 min



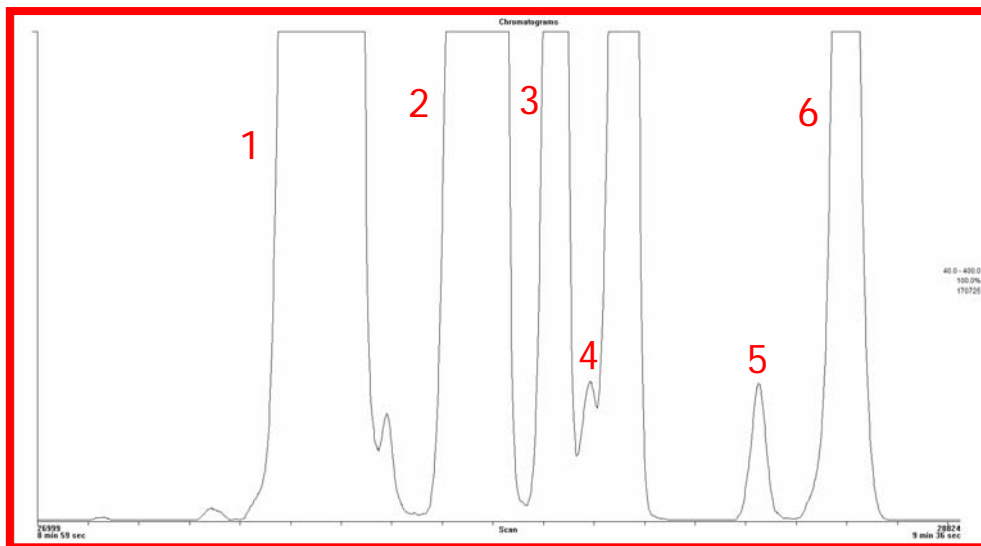


### ISO E SUPER REGION EXPANSION

1	hedione
2	iso E super (isomer 1)
3	iso E super (isomer 2)
4	salicylate hexile
5	hedione (isomer)
6	iso E super (isomer 3)

### AUTOMATIC DECONVOLUTION RESULTS

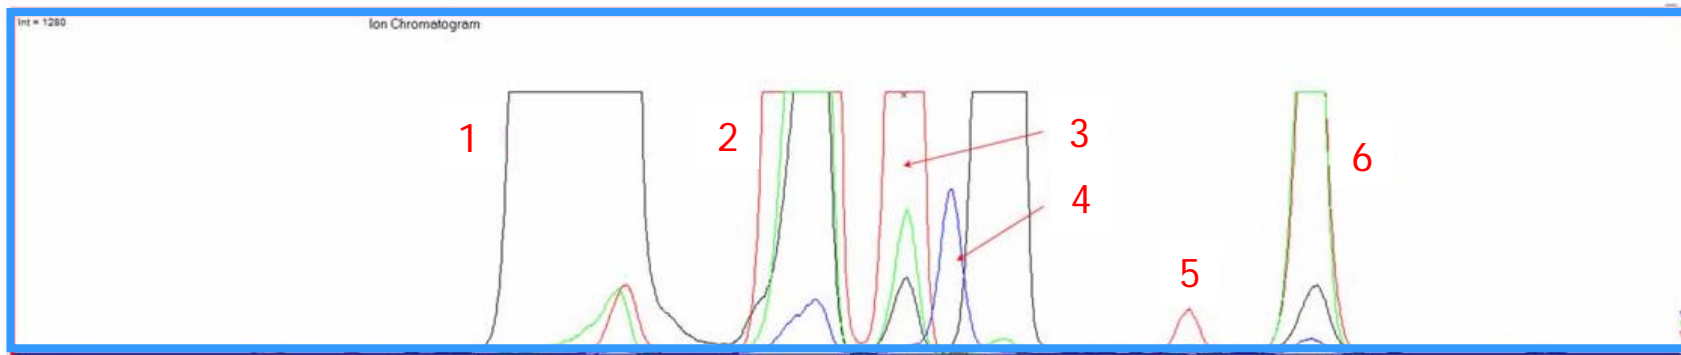

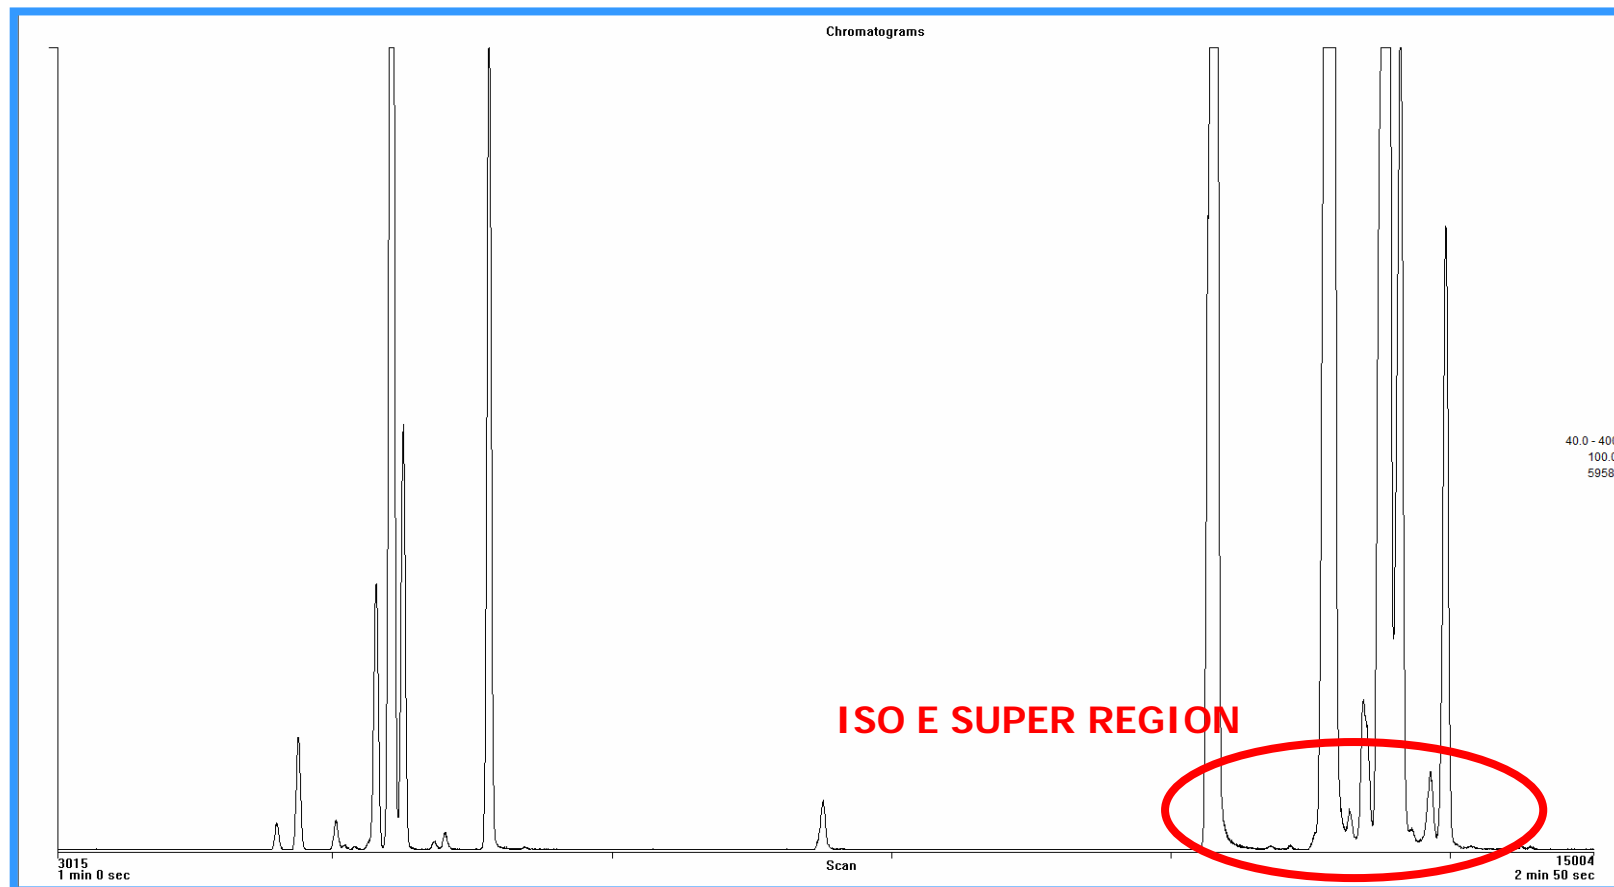


### Gas Chromatograph

Injector: Split-Splitless  
Injector Temperature: 250°C  
Injector Volume: 0.5 µl  
Split Ratio: 1:800  
Column: DN-5 3 m x 0.1 mm, 0.1 µm  
Linear Velocity: 40 cm/sec at constant linear velocity  
Oven Temperature Program: from 100°C to 250°C at 50°C/min

### Time of Flight




Transfer line temperature: 220°C  
Sampling rate: 100 Hz  
Mass range: 40-400 amu  
Solvent delay: 60 sec  
Acquisition time: 3 min

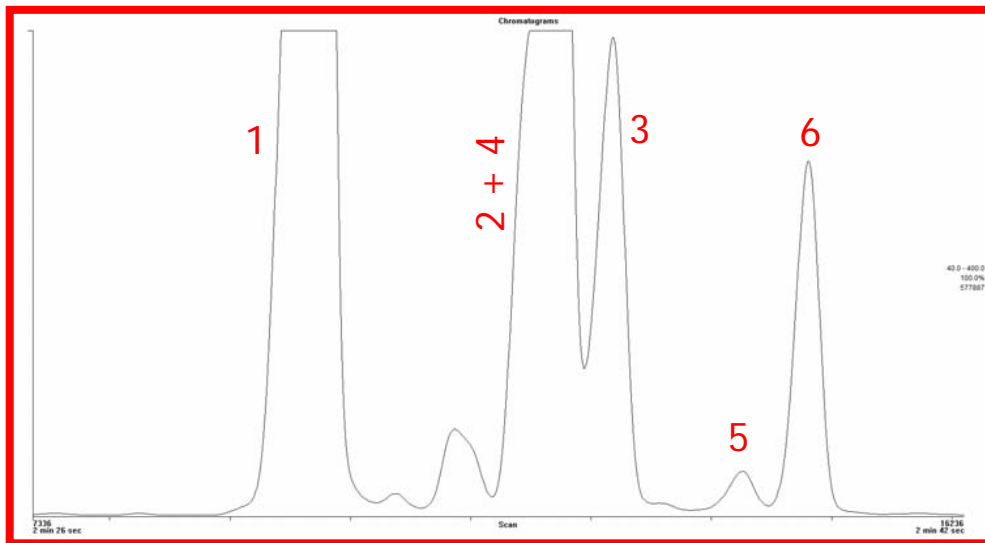

### ISO E SUPER REGION EXPANSION




1	hedione
2	iso E super (isomer 1)
3	iso E super (isomer 2)
4	salicylate hexile
5	hedione (isomer)
6	iso E super (isomer 3)

### AUTOMATIC DECONVOLUTION RESULTS

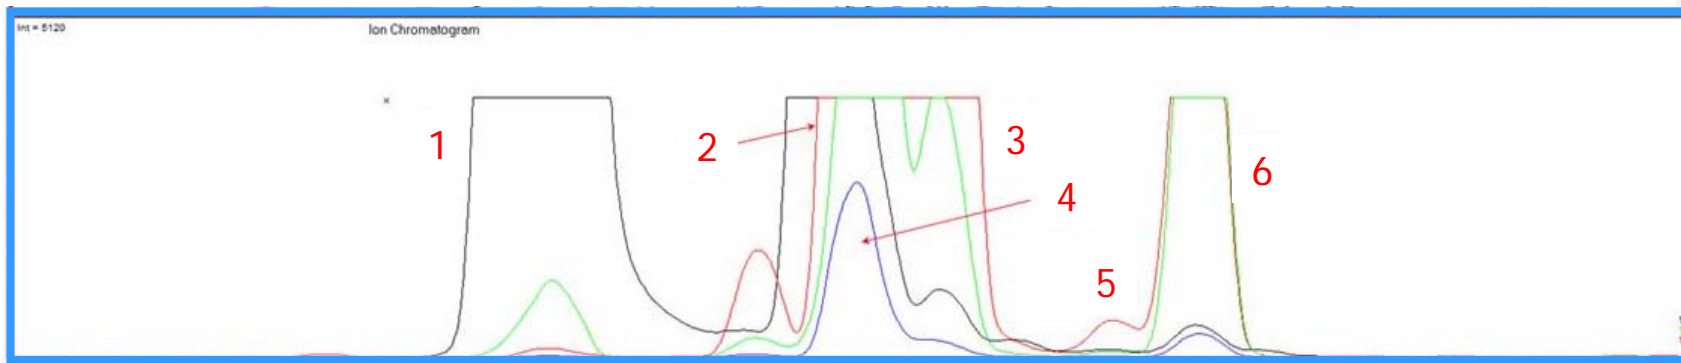

# Master TOF Time of Flight Mass Spectrometer APPLICATIONS

Fast GC with Short Micro Bore Column

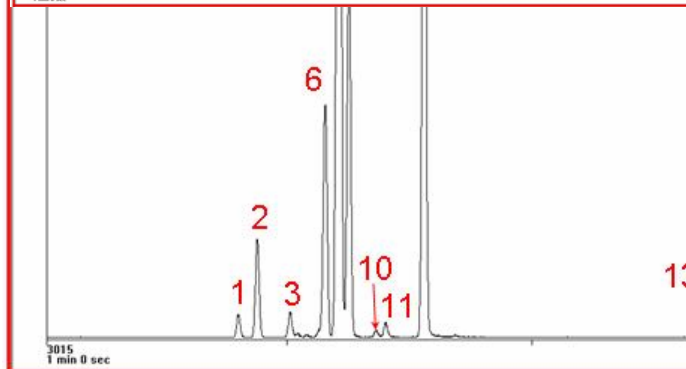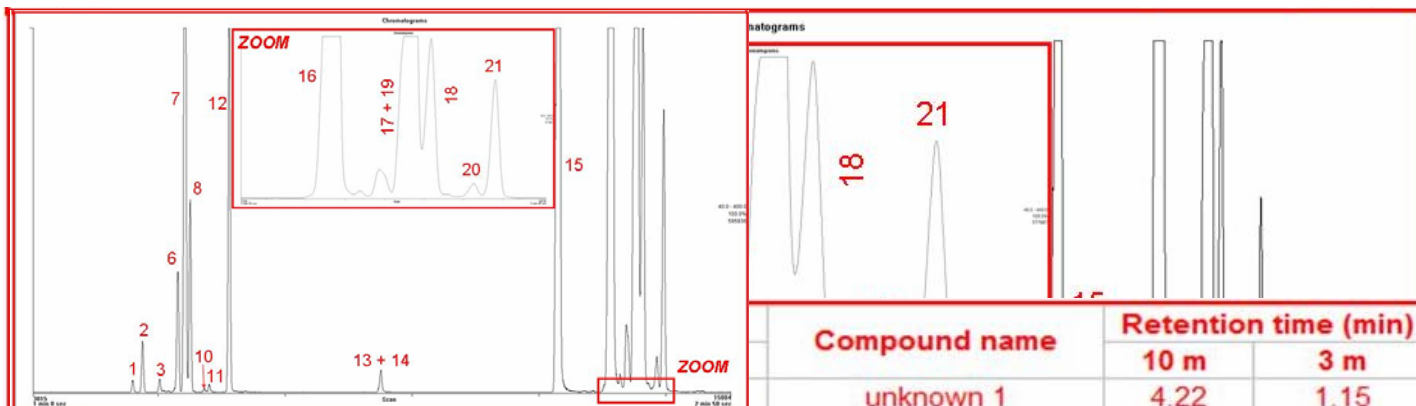



	Compound name	Retention time (min)		Masses
		10 m	3 m	
	unknown 1	4.22	1.15	-
2	$\beta$ -terpineol, -cis	4.28	1.17	71, 93, 136
3	$\beta$ -terpineol, -trans	4.40	1.20	71, 93, 136
4	unknown 2	4.42	-	-
5	unknown 3	11.45	-	-
6	acetate styrallyle	4.57	1.23	122, 104, 164
7	$\alpha$ -terpineol	4.57	1.24	59, 93, 121
8	$\gamma$ -terpineol	5.01	1.25	121, 93, 154
9	unknown 4	5.18	-	-
10	nerol	-	1.27	69, 84, 93
11	citronellol	-	1,28	69, 95, 156
12	acetate linalyle	5.34	1.31	93, 80, 136
13	jasmone, trans-	6.58	1.55	79, 91, 164
14	vanilline	6.58	1.55	151, 81, 109
15	diethyl phtalate	8.41	2.23	149, 177, 222
16	hedione	9.12	2.31	83, 156, 226
17	iso E super (isomer 1)	9.17	2.35	191, 135, 219
18	iso E super (isomer 2)	9.20	2.36	135, 191, 219
19	salicylate hexile	9.21	2.35	120, 138, 222
20	hedione (isomer)	9.23	2.34	83, 156, 226
21	iso E super (isomer 3)	9.31	2.39	135, 191, 219



## DETERMINATION of ALLERGENES in COSMETIC PRODUCTS

In the 7th Amendment to the European Cosmetics Directive, the Scientific Committee for Cosmetics & Non-Food Products (SCCNFP) established a list of components as being responsible, or suspected to be, of a series of skin allergies. According to the aforementioned regulation the maximum residue limit for “leave-on” and “rinse-off” cosmetic products is fixed at 0.001% and 0.01%, respectively. The regulation foresees that any allergen, present in excess must be reported on the product label.






### SCCNFP Allergens List

Limonene	Citral (Geranial)	Isoeugenol	Hexyl cinnamaldehyde
Benzyl alcohol	Cinnamic aldehyde	$\alpha$ -isomethylionone	Benzyl benzoate
Linalool	Anysil Alcohol	Lilial	Benzyl salicylate
Methyl 2-octynoate	Hydroxycitronellal	Amyl cinnamal	Benzyl cinnamate
Citronellol	Cinnamyl alcohol	Lyral	oak moss
Citral (Neral)	Eugenol	Amylcinnamil alcohol	tree moss
Geraniol	Coumarin	Farnesol	

*..... 24 are volatiles.*

# ALLERGENS DETERMINATION IN COSMETIC PRODUCTS

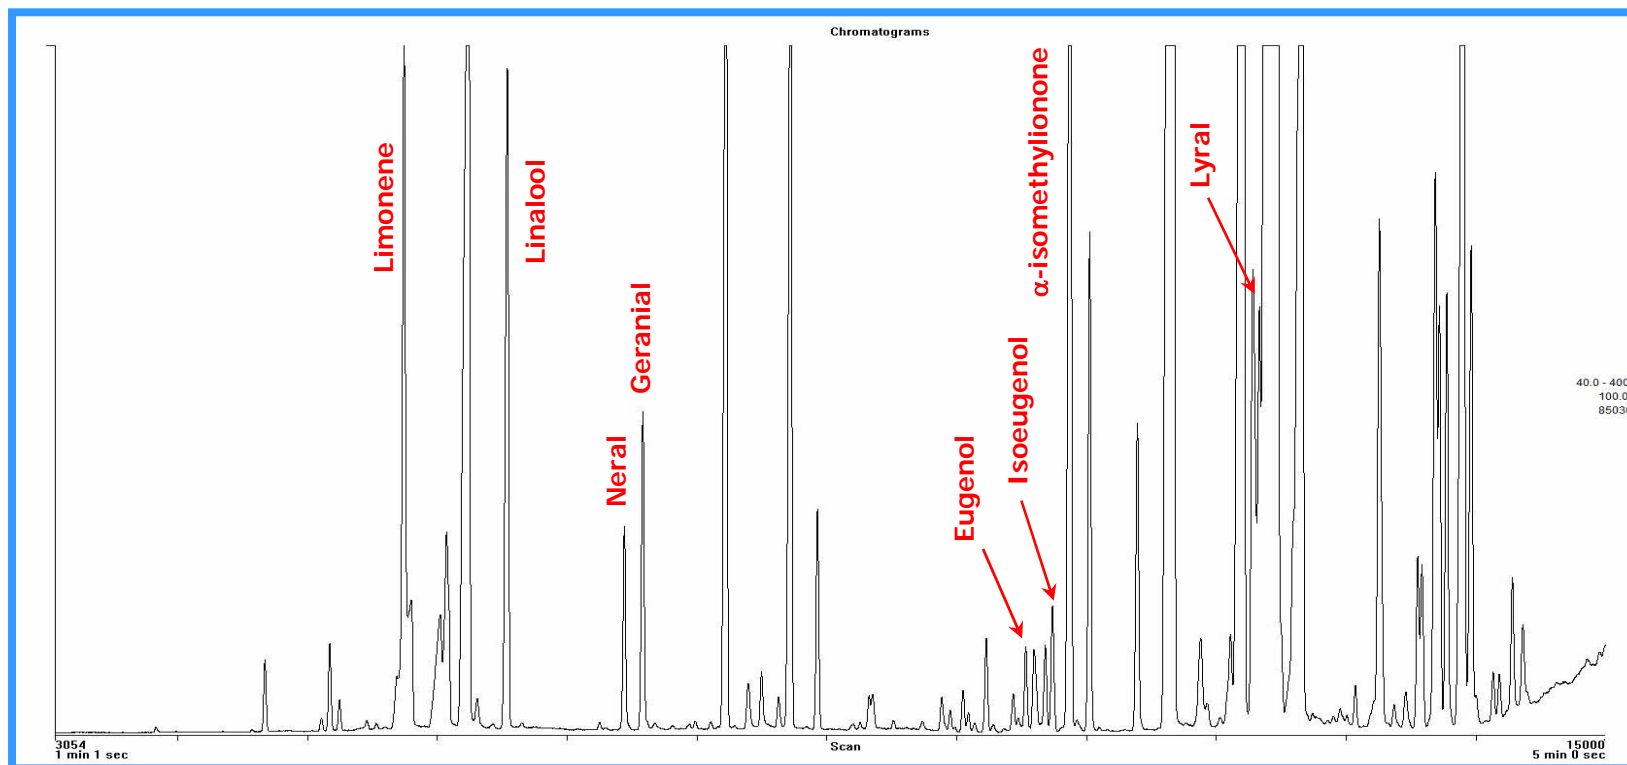

## Gas Chromatograph

Injector: Split-Splitless

Injector Temperature: 250°C

Injector Volume: 1.0 µl

Split Ratio: 1:20

Column: DN-5 10 m x 0.1 mm, 0.1 µm

Linear Velocity: 40 cm/sec at constant linear velocity

Oven Temperature Program: from 50°C to 250°C at 40°C/min

## Time of Flight

Transfer line temperature: 220°C

Sampling rate: 50 Hz




Mass range: 40-400 amu

Solvent delay: 60 sec

Acquisition time: 5 min

Perfume  
Analysis

# ALLERGENES DETERMINATION IN COSMETIC PRODUCTS

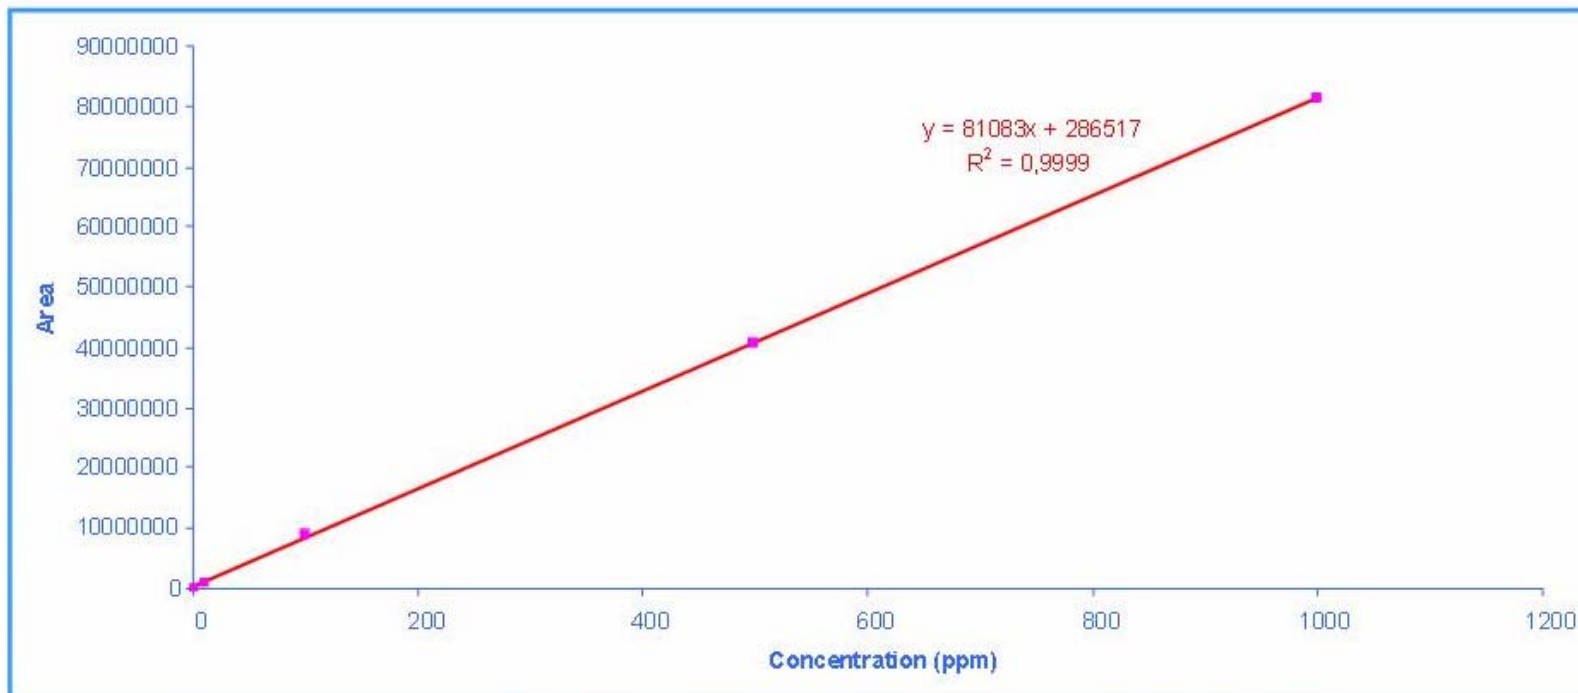

*Limonene calibration plot in the range 1 to 1000 ppm*

ALLERGEN	Quant. Mass	ppm
Limonene	68	98
Linalool	93	82
Citral (Neral)	69	60
Citral (Geranial)	69	43
Eugenol	164	40
Isoeugenol	164	52
$\alpha$ -isomethylionone	206	280
Lyrar	192	97

*Quantitative Results of 8 Allergenes determined in the perfume*

## TruTOF HT



**Mass Range:**

**Acquisition Speed:** up to 80 spectra/s

**GC/MS Ion Source:** EI (standard) and CI (optional)

**Sensitivity:** 2 pg Hexachlorobenzene s/n 10:1

**Linearity:**  $10^4$


**Resolution:** N.D.

**Pumps:**

**Software:** Total Control MS TOF, GC7890 and AS

**Library:** NOT COMPATIBLE NIST

## Pegasus HT

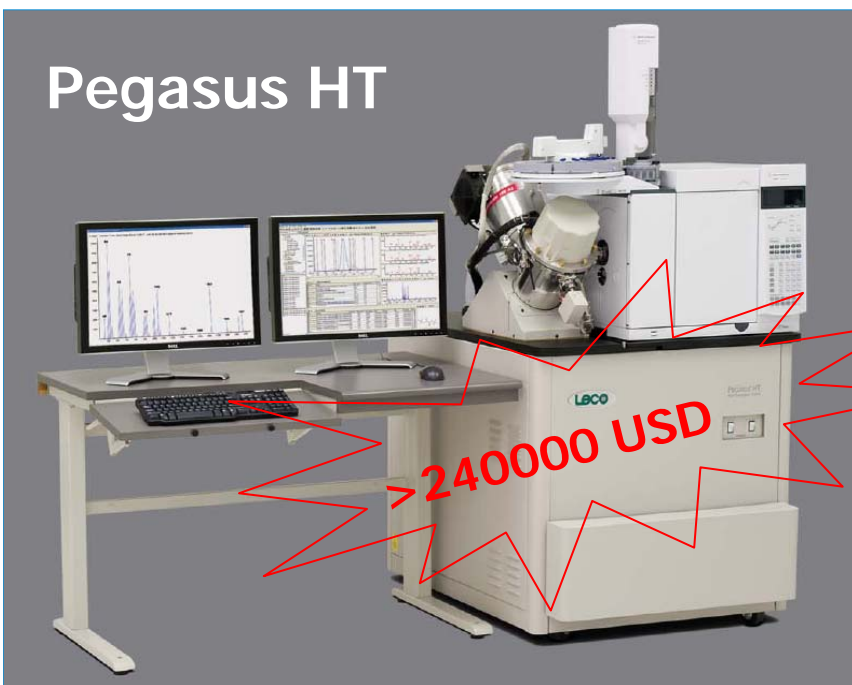

**Mass Range:** up to 1000

**Acquisition Speed:** up to 500 spectra/s

**GC/MS Ion Source:** EI (standard) and CI (optional)

**Sensitivity:** 2 pg Hexachlorobenzene s/n 10:1

**Linearity:**  $10^4$

**Resolution:** N.D.

**Pumps:**

**Software:** Total Control MS TOF, GC7890 and AS

**Library:** NOT COMPATIBLE NIST



MASTER TOF – Competitors

# Master TOF Time of Flight Mass Spectrometer

## Specifications




<b>Mass Range</b>	5 to 1500 amu
<b>Acquisition rate</b>	Up to 1000 spectra/s
<b>Sensitivity</b>	1 pg Octafluoronaphthalene s/n > 10:1 at m/z 272
<b>Resolution</b>	1500
<b>Linearity</b>	10 <sup>5</sup>
<b>Tune mode</b>	Automatic Full Autotune Automatic Autotune Manual Tune
<b>Ion Source</b>	EI – Standard CI (+/-) Optional
<b>Vacuum System</b>	Internal Diaphragm Pump 2 Turbomolecular pumps 260-70 L/s

**130000 Euro**





*... the MASTER TOF GC/MS system offers ...*

- ... a **complete solution**, starting from the injector, passing through the GC oven and the detector up to the software
- ... the **appropriate acquisition** for MS detection in FastGC and GCXGC..
- ... all in a **reduced bench space**..
- ... at a strongly **competitive price**



## *DANI Chromatographic Products*

- GC and GC/MS
- Automatic samplers for GC





**MASTER TD – Thermal Desorber**



## ... *low analysis costs & improved sensitivity*


As an alternative method to traditional solvent extraction, **Master TD** offers:

- up to 1000-10000 times increase in sensitivity
- higher recovery (over 95% for all volatile substances)
- minimal sample handling and the reuse of the sampling tubes
- total reduction of cost/sample
- easy connection to any kind of GC

## ... *high sample throughput*

**MASTER TD** operates automatically from thermal extraction to injection to maximize the laboratory productivity. It includes:

- a **50-place carousel** for standard ¼" x 3.5 inch tubes
- **cryogen-free trap cooling** (down to -40°C) for continuous and unattended operation
- **overlapping mode** - desorption of a subsequent sample begins while GC analysis of a previous sample continues



## ... *two stage Thermal Desorber*

**MASTER TD** excellent analytical performances are provided through:




- a **two-stage thermal desorption** process - the compounds are desorbed from the sample tube by heating in a flow of inert gas and refocused in a narrow-bore packed trap kept a low temperature
- **instant trap desorption** (Patented) to introduce the components in a narrow band directly into the analytical column through a heated transfer line
- extended range of application from volatile to semi-volatile compounds **up to C44** boiling point equivalent
- completely **inert** sample path
- **cryogen-free trap cooling** down to -40°C for efficient trapping of very volatile compounds (from C2, CFC,..)
- optional ***Air Sampler*** device for on-line monitoring
- Simple and intuitive ***Control Manager*** software





## *Master TD Thermal Desorber*

### *Fields of Applications*


- **VOCs in Ambient**  
BTEX; Chlorinated hydrocarbons; 1,3-butadiene;  
Ozone Precursors; Formaldehyde; Acrylonitrile;
- **Indoor Air Pollution**  
Building products; Cleaning agents; Air conditioning;
- **Emission Monitoring**  
Stack emissions; Industrial emissions;
- **Products Quality Control**  
Residual solvents; Pharmaceutical; Food packaging;  
Food Industry;
- **Workplace Monitoring**  
Styrene; Ethylene oxide; plastics; polymers;



## Master TD Thermal Desorber



## VOCs - BTEX analysis

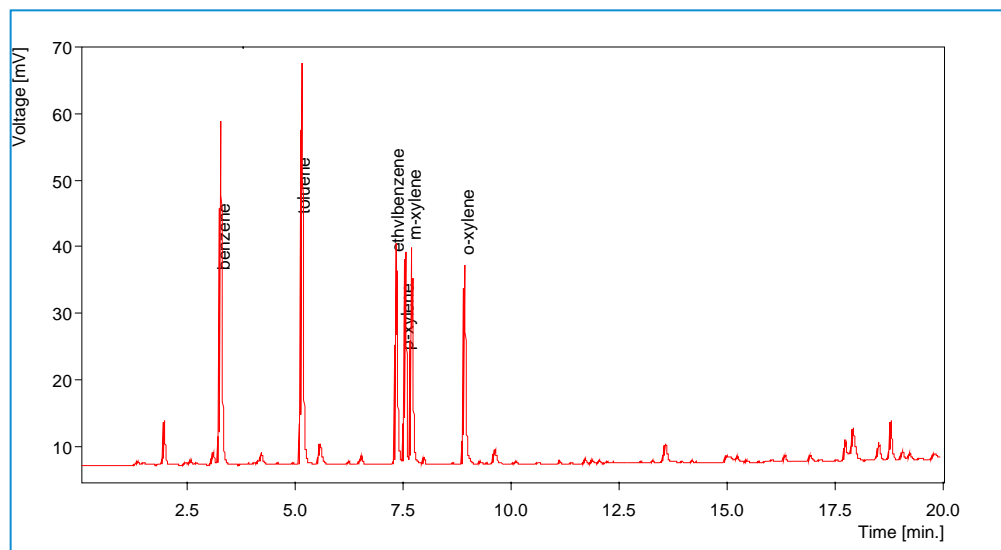

### GC Conditions

**Column:** Carbowax 30m, 0,32mm

**Inj:** SL/IN 350°C

**Det:** FID 350°C

**Carrier:** He

### TD Conditions

**Trap:** Tenax GR

**Tube:** Tenax GR

**Sample Volume:** 1000ml


**Minimum detectable level:** 0.1ppm

## Repeatability on 10 replicates

	Benzene	Toluene	Ethylbenzene	p-Xylene	m-Xylene	o-Xylene
<b>Average</b>	8,05	8,04	8,03	8,06	8,03	8,17
<b>St.dev.</b>	0,06	0,09	0,07	0,09	0,10	0,09
<b>RSD%.</b>	<b>0,70</b>	<b>1,09</b>	<b>0,86</b>	<b>1,13</b>	<b>1,20</b>	<b>1,10</b>

## Master TD Thermal Desorber

### VOCs - Chlorinated hydrocarbons analysis

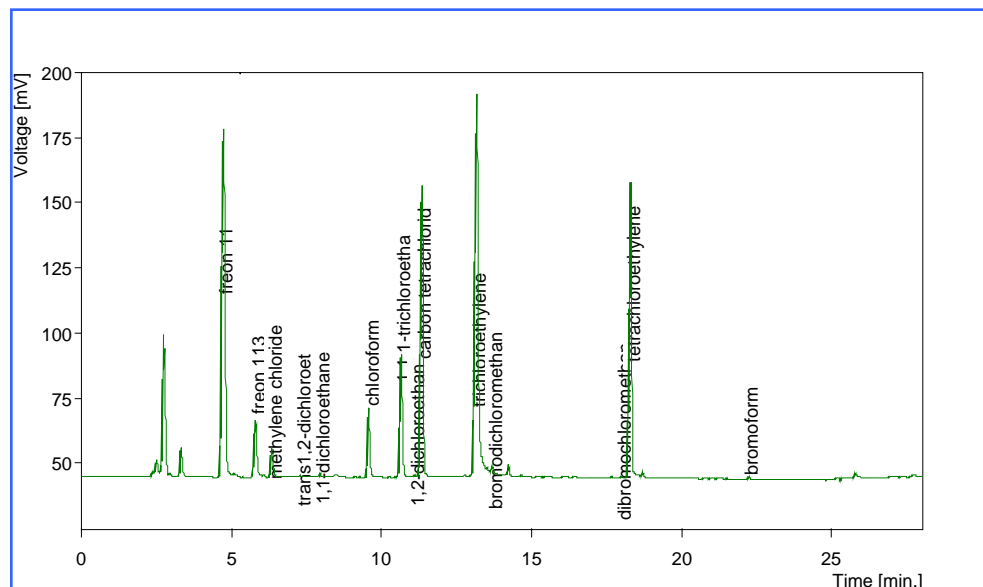

#### GC Conditions

**Column:** DB624, 60m, 0,32mm

**Inj:** SL/IN 350°C

**Det:** ECD 350°C

**Carrier:** He

#### TD Conditions

**Trap:** CarboxpackB-Carboxieve SIII


**Tube:** CarboxpackB-Carboxieve SIII

**Sample Volume:** 250ml


**Minimum detectable level:** ppt

#### Repeatability on 10 replicates

	CFC11	CFC113
<b>Average</b>	1011,8	395,6
<b>Std. Dev.</b>	17,7	3,5
<b>RSD%</b>	<b>1,8</b>	<b>0,9</b>



<b>Desorption Mode</b>	Two-Stage
<b>Sample Tube Capacity</b>	50
<b>Tube Temperature Range</b>	40 to 400°C
<b>Dry-step</b>	YES
<b>Trap Desorption Flow</b>	Back Flush
<b>Trap Cooling system</b>	Electrically powered Peltier
<b>Trap Low temperature</b>	-40°C
<b>Trap High temperature</b>	450°C
<b>Trap Heating rates</b>	"instant heating"
<b>Transfer Line Temperature range</b>	50 to 290°C
<b>Valve Temperature range</b>	50 to 300°C
<b>Valve</b>	Electrically actuated
<b>Tube Leak test</b>	YES
<b>Trap Leak test</b>	YES
<b>Volatility Range</b>	C2-C44
<b>Sample Flow path</b>	inert deactivated Siltek®
<b>Compatibility</b>	any kind of GC or GC/MS
<b>ON-LINE sampling</b>	YES (10 lines)





**MASTER DHS – Dynamic Headspace Sampler**


## *... analysis of VOCs in liquid and solid*

Master DHS allows the recovery of VOCs at low detection limits in both liquid and solid samples on the same instrument:

- Environmental applications (water, wastewater, sludge, soil)
- Q.C. applications in:
  - Flavour and fragrances (spices, herbs, foods, soaps);
  - Chemicals (plastics, papers,..);
  - Pharmaceutical (residual solvents).



## *... flexible and extended automation*

- 18-seat internal vial carousel
- sample capacity extended to 65 vials with MasterAS
- sample overlapping minimizes overall analysis time
- precise external addition of IS, surrogates, spiking solution, reagents..





# Master DHS Dynamic Head Space Sampler





2 solvent vials,  
2 waste vials

6 vials for internal standard, surrogates,  
spiking solution


65-seat sample tray

## ... enhanced sensitivity & easy sample management

- VOCs are purged/stripped and focused on a packed trap for the maximum sensitivity
- easy and convenient sample preparation using standard 20 ml HS vials
- no cross-contamination

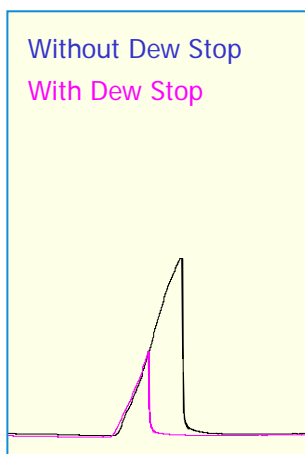
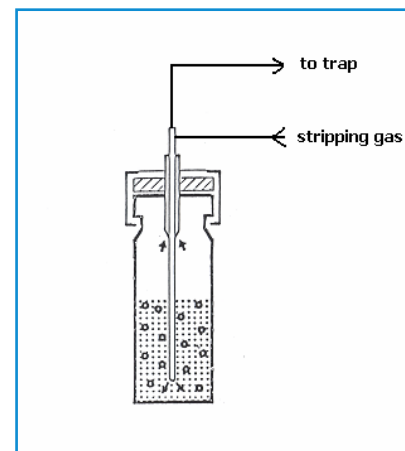


Humidity


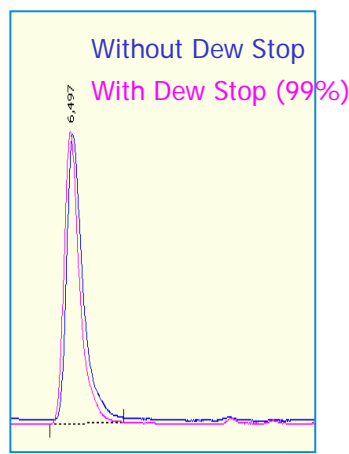


Propanol



- “Dew Stop” removes most of the humidity keeping the volatiles unaffected
- completely inert sample path preserves sample integrity



# Master DHS Dynamic Headspace

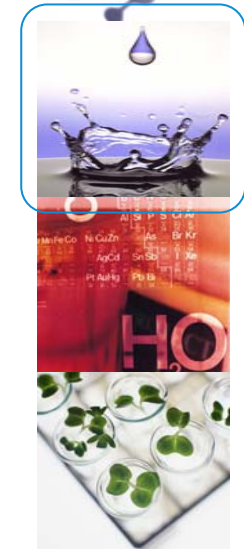



## Chlorinated hydrocarbons in water

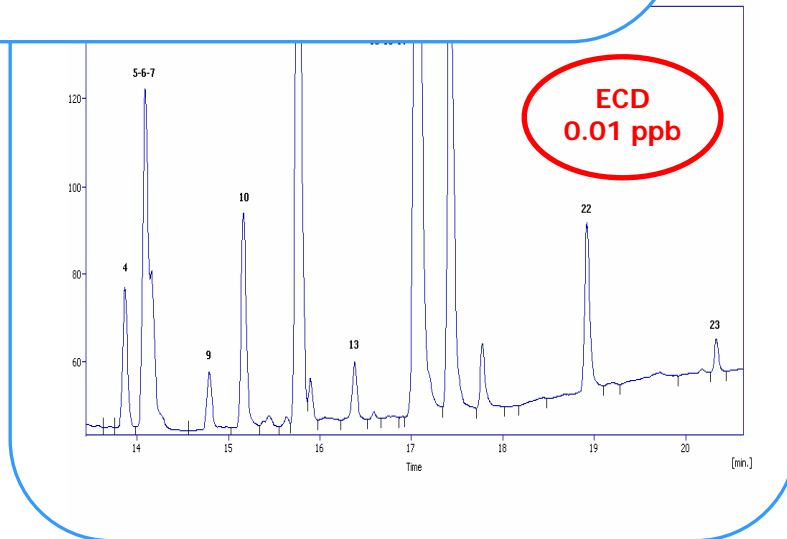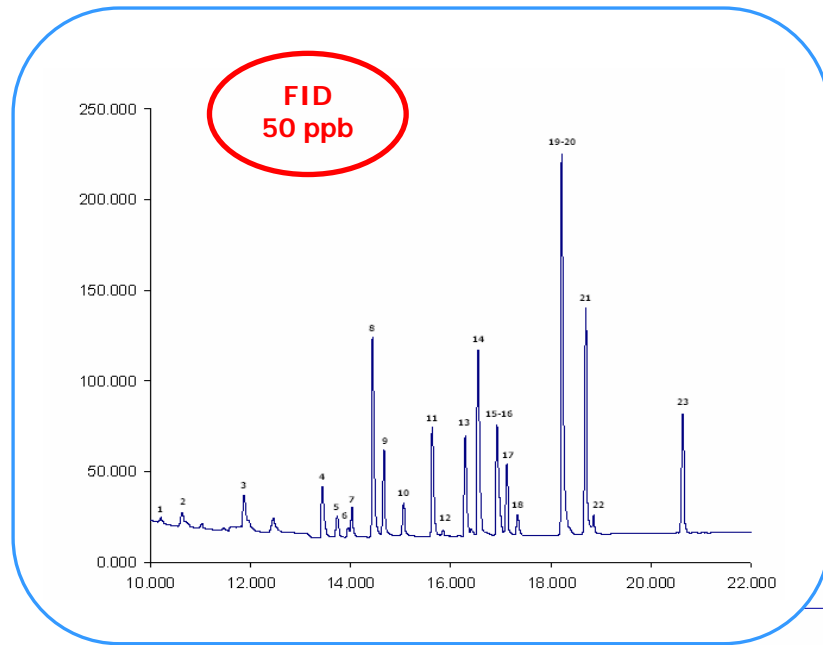

1	1,1-Dichlorethene
2	Methylene Chloride
3	<i>trans</i> -1,2- Dichloroethene
4	<i>cis</i> -1,2- Dichloroethene
5	Chloroform
6	Carbon Tetrachloride
7	1,1,1-Trichloroethane
8	Benzene
9	1,2-Dichloroethane
10	Trichloroethene
11	1,2-Dichloropropane
12	Bromodichloromethane
13	<i>cis</i> -1,3-Dichloropropene
14	Toluene
15	<i>trans</i> -1,3-Dichloropropene
16	Tetrachloroethane
17	1,1,2-Trichloroethane
18	Dibromochloromethane
19	<i>m</i> -Xylene
20	<i>p</i> -Xylene
21	<i>o</i> -Xylene
22	Bromoform
23	1,4-Dichlorobenzene

<b>Operating Principle</b>	Two stage dynamic head space
<b>Capacity</b>	65 vials
<b>Sampling Vials</b>	20ml sample vial
<b>Incubation oven capacity</b>	18 vials
<b>Incubation oven temperature</b>	Amb.- 250°C
<b>Overlapping sample processing</b>	Yes
<b>Focusing Trap</b>	Quartz packed
<b>Trap Temperature</b>	Amb. - 450°C
<b>Desorption Time</b>	From 0 up to 999.9 min, 0,1 min resolution
<b>Trap Heating</b>	1000°C/min direct heating
<b>Transfer Line Temperature</b>	50°C - 300°C
<b>Sampling Valve Temperature</b>	50°C - 300°C
<b>Sample Flow-path</b>	Siltek®
<b>Water Removal</b>	Yes (Dew Stop)
<b>Solvent/ IS addition</b>	2 solvent, 2 waster vials 6 standard vials
<b>Compatibility</b>	Each kind of GC or GC/MS





**HSS 86.50 – Static Headspace Sampler**

## *... the most reliable sampling technique*


Static headspace technique offers many advantages

- Little or no sample preparation
- Higher sensitivity
- No solvent peak
- Column life increase

## *... the most reliable automatic sampler*

HSS 86.50 offers the highest precision and repeatability (RSD% < 1%) through

- **accurate** temperature and pressure control
- **constant** incubation time
- **Valve&Loop** sampling technique, introducing a highly repeatable gas volume
- no risk of condensation, no influence on carrier gas flow/pressure



## ... *sample integrity & negligible carryover*


- the **chemical inertness** of the sample path
- the **low dead volumes** and
- the **constant washing** flow of the sample path

provide absolutely negligible levels of contamination and unaffected sample integrity

## ... *high sample throughput*





**HSS 86.50** features

- up to **44 samples** in 20 or 10 ml vials
- sample overlapping of up to 12 vials to optimise analysis times for high productivity






*... HSS 86.50 applies to*

- **Plastic industry**  
Acetaldehyde determination in polymers
- **Pharmaceutical industry**  
Residual volatile solvents in pharmaceutical
- **Food industry**  
Flavours in food
- **Industrial quality control**  
Ethylene oxide in sterilized products
- **Environmental**  
Volatile pollutants in water and soil

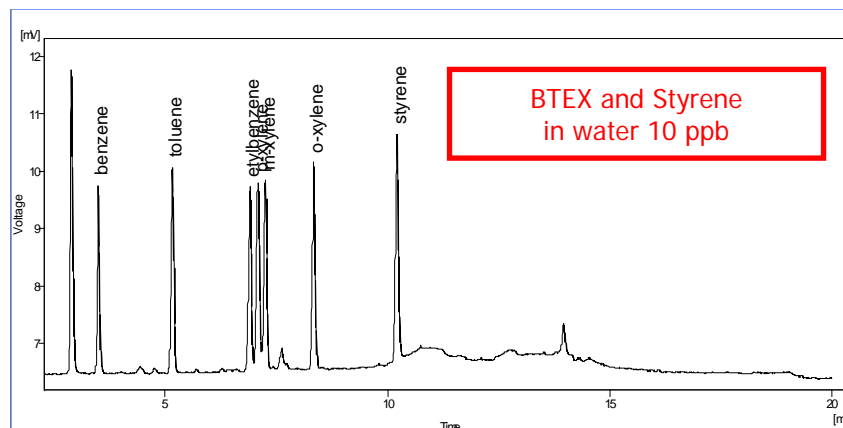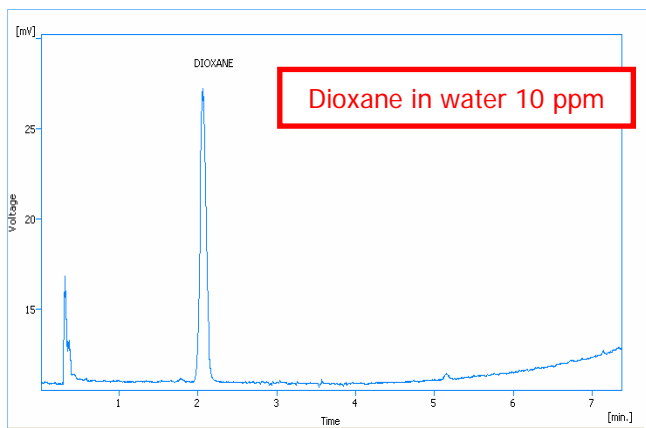



<b>Sampling Method</b>	Valve & Loop
<b>Sample Loops</b>	1 ml standard (0.5 and 3 ml optional)
<b>Sample Flow Path</b>	Siltek®
<b>Sample Capacity</b>	44 vials
<b>Vials</b>	20ml or 10ml
<b>Sampling device temperature</b>	from 50°C to 220°C
<b>Incubation Oven Capacity</b>	6 vials
<b>Incubation Oven Temperature</b>	from 40°C to 200°C
<b>Constant Heating Time</b>	YES
<b>Sample Shaking</b>	YES (fast and slow)
<b>Overlapping sample processing</b>	YES
<b>Transfer Line Temperature</b>	from 50°C to 220°C
<b>Transfer Line material</b>	Siltek®
<b>MHE (Multiple Headspace Extraction)</b>	YES, 10 steps each vials
<b>Compatibility</b>	any kind of GC or GC/MS



**По вопросам продажи и поддержки обращайтесь:**

**Архангельск** (8182)63-90-72  
**Астана** (7172)727-132  
**Астрахань** (8512)99-46-04  
**Барнаул** (3852)73-04-60  
**Белгород** (4722)40-23-64  
**Брянск** (4832)59-03-52  
**Владивосток** (423)249-28-31  
**Волгоград** (844)278-03-48  
**Вологда** (8172)26-41-59  
**Воронеж** (473)204-51-73  
**Екатеринбург** (343)384-55-89  
**Иваново** (4932)77-34-06  
**Ижевск** (3412)26-03-58  
**Казань** (843)206-01-48

**Калининград** (4012)72-03-81  
**Калуга** (4842)92-23-67  
**Кемерово** (3842)65-04-62  
**Киров** (8332)68-02-04  
**Краснодар** (861)203-40-90  
**Красноярск** (391)204-63-61  
**Курск** (4712)77-13-04  
**Липецк** (4742)52-20-81  
**Магнитогорск** (3519)55-03-13  
**Москва** (495)268-04-70  
**Мурманск** (8152)59-64-93  
**Набережные Челны** (8552)20-53-41  
**Нижний Новгород** (831)429-08-12  
**Новокузнецк** (3843)20-46-81

**Новосибирск** (383)227-86-73  
**Омск** (3812)21-46-40  
**Орел** (4862)44-53-42  
**Оренбург** (3532)37-68-04  
**Пенза** (8412)22-31-16  
**Пермь** (342)205-81-47  
**Ростов-на-Дону** (863)308-18-15  
**Рязань** (4912)46-61-64  
**Самара** (846)206-03-16  
**Санкт-Петербург** (812)309-46-40  
**Саратов** (845)249-38-78  
**Севастополь** (8692)22-31-93  
**Симферополь** (3652)67-13-56  
**Смоленск** (4812)29-41-54

**Сочи** (862)225-72-31  
**Ставрополь** (8652)20-65-13  
**Сургут** (3462)77-98-35  
**Тверь** (4822)63-31-35  
**Томск** (3822)98-41-53  
**Тула** (4872)74-02-29  
**Тюмень** (3452)66-21-18  
**Ульяновск** (8422)24-23-59  
**Уфа** (347)229-48-12  
**Хабаровск** (4212)92-98-04  
**Челябинск** (351)202-03-61  
**Череповец** (8202)49-02-64  
**Ярославль** (4852)69-52-93

**Единый адрес для всех регионов:** [drs@nt-rt.ru](mailto:drs@nt-rt.ru) || [www.danimaster.nt-rt.ru](http://www.danimaster.nt-rt.ru)